

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048308.D
 Acq On : 30 Oct 2024 05:11
 Operator : RC/JU
 Sample : PB164512BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK512

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	36	rBV	72401	89135	2.21%	0.184%
2	3.581	97	101	117	rBV	812663	1244785	30.89%	2.573%
3	3.910	153	157	163	rVB2	17969	28176	0.70%	0.058%
4	6.892	654	664	677	rBV	875437	1444633	35.85%	2.986%
5	7.045	684	690	703	rVB	731347	1209988	30.03%	2.501%
6	7.251	718	725	740	rVB	917250	1498798	37.20%	3.098%
7	7.716	797	804	818	rBV	764142	1268538	31.48%	2.622%
8	7.939	839	842	846	rVB5	2760	4545	0.11%	0.009%
9	8.428	918	925	938	rBV	1058957	1778562	44.14%	3.677%
10	8.869	993	1000	1015	rBV	839308	1417118	35.17%	2.930%
11	9.292	1068	1072	1077	rVB2	13312	20497	0.51%	0.042%
12	9.592	1116	1123	1138	rBV	683341	1167923	28.98%	2.414%
13	10.133	1206	1215	1226	rBV	955970	1712204	42.49%	3.540%
14	10.504	1270	1278	1287	rBV	1094217	1845841	45.81%	3.816%
15	10.645	1294	1302	1322	rBV	857140	1728937	42.91%	3.574%
16	11.786	1492	1496	1502	rVB3	12197	18384	0.46%	0.038%
17	12.122	1546	1553	1559	rBV3	13863	25868	0.64%	0.053%
18	13.221	1735	1740	1744	rBV8	2026	4082	0.10%	0.008%
19	13.769	1826	1833	1850	rBV	1660084	2399323	59.55%	4.960%
20	14.051	1873	1881	1897	rBV	2005488	2998087	74.41%	6.198%
21	14.357	1924	1933	1942	rBV	1587422	2328191	57.78%	4.813%
22	14.580	1964	1971	1998	rBV	338491	904980	22.46%	1.871%
23	15.351	2095	2102	2116	rBV	2425580	3560082	88.35%	7.360%
24	15.480	2118	2124	2140	rVV	594688	916383	22.74%	1.894%
25	15.592	2140	2143	2147	rVB2	12803	20147	0.50%	0.042%
26	15.874	2188	2191	2194	rBV6	3489	4356	0.11%	0.009%
27	16.245	2251	2254	2260	rVB7	3484	4793	0.12%	0.010%
28	16.604	2308	2315	2319	rBV7	4534	9676	0.24%	0.020%
29	16.886	2359	2363	2368	rBV3	4540	7425	0.18%	0.015%
30	17.098	2393	2399	2409	rBV	1757066	2470612	61.31%	5.107%
31	17.198	2410	2416	2438	rVB	2498514	3669980	91.08%	7.587%
32	17.656	2491	2494	2500	rBV7	4984	8335	0.21%	0.017%
33	19.056	2728	2732	2740	rBV5	25750	40066	0.99%	0.083%
34	19.133	2740	2745	2751	rBV2	26368	45174	1.12%	0.093%
35	19.492	2800	2806	2818	rBV	2873415	4029405	100.00%	8.330%
36	21.321	3112	3117	3131	rBV	1469867	2353244	58.40%	4.865%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048308.D
Acq On : 30 Oct 2024 05:11
Operator : RC/JU
Sample : PB164512BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK512

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	24.062	3575	3583	3595	rBV	1547264	3640475	90.35%	7.526%
38	24.268	3610	3618	3632	rVB	958559	2453833	60.90%	5.073%




Sum of corrected areas: 48372581

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048308.D
Acq On : 30 Oct 2024 05:11
Operator : RC/JU
Sample : PB164512BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK512

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

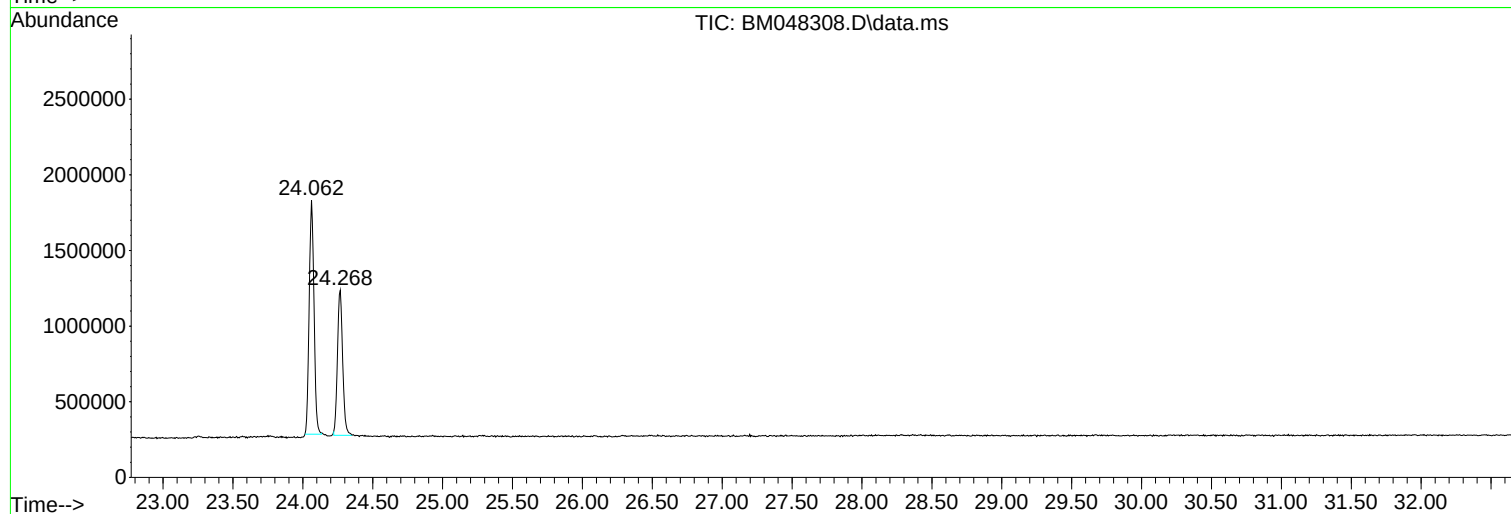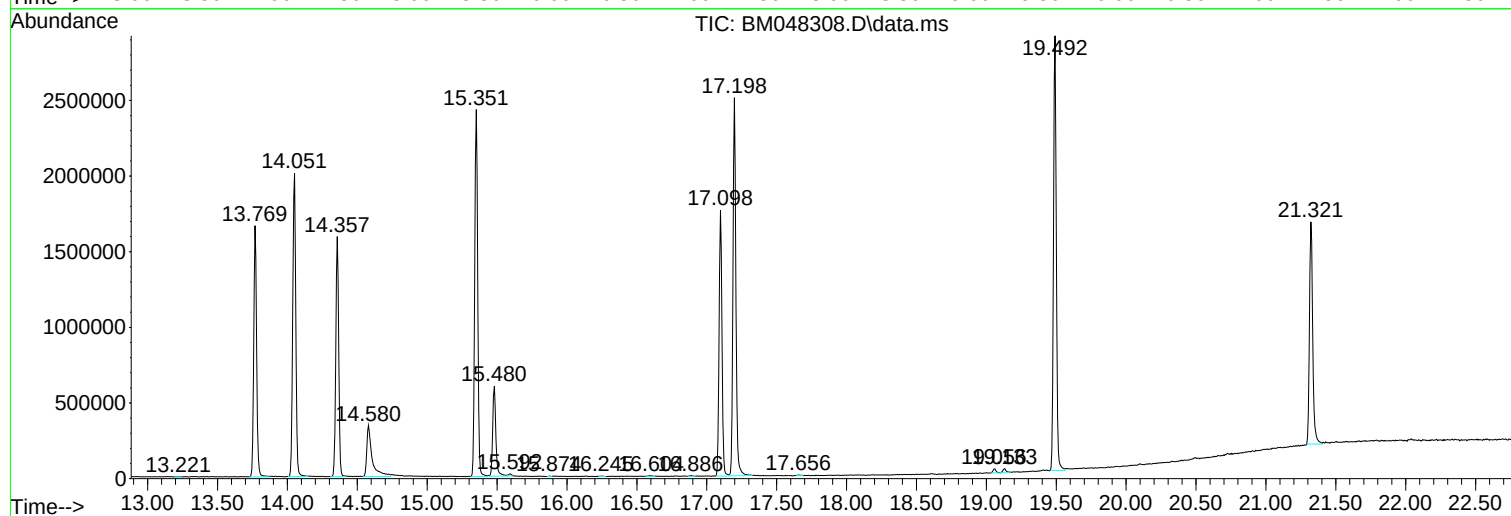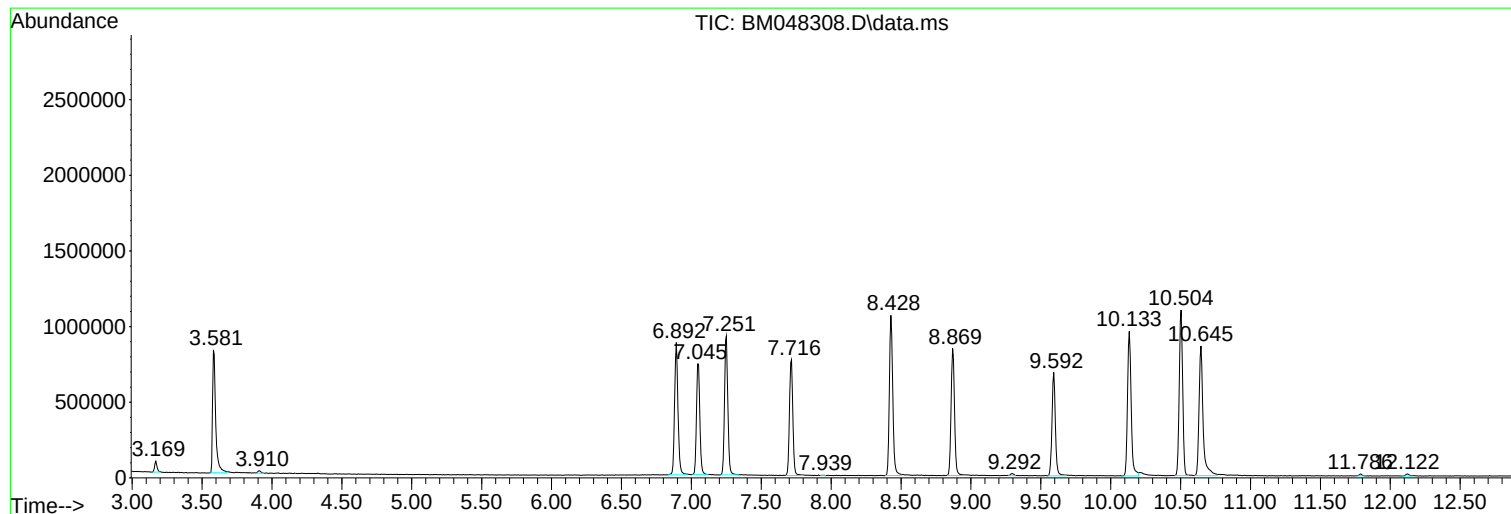

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048308.D
Acq On : 30 Oct 2024 05:11
Operator : RC/JU
Sample : PB164512BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK512

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048308.D
Acq On : 30 Oct 2024 05:11
Operator : RC/JU
Sample : PB164512BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK512

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc