

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048309.D
 Acq On : 30 Oct 2024 05:50
 Operator : RC/JU
 Sample : PB164514BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK514

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048309.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	39	rVB	71977	90535	2.27%	0.193%
2	3.581	98	101	119	rBV	826068	1251749	31.40%	2.675%
3	3.910	153	157	162	rVB	17109	23918	0.60%	0.051%
4	6.893	655	664	675	rBV	851676	1401075	35.14%	2.994%
5	7.045	684	690	699	rBV	727183	1173383	29.43%	2.508%
6	7.251	718	725	736	rBV	881725	1472669	36.94%	3.147%
7	7.381	746	747	752	rVB5	4304	4759	0.12%	0.010%
8	7.710	796	803	813	rBV	710997	1191200	29.88%	2.546%
9	8.304	898	904	907	rVB7	2905	4702	0.12%	0.010%
10	8.428	918	925	947	rBV	1031381	1740062	43.64%	3.719%
11	8.869	993	1000	1014	rBV	812316	1378711	34.58%	2.947%
12	9.298	1068	1073	1079	rVB5	9261	14483	0.36%	0.031%
13	9.592	1115	1123	1137	rBV	667094	1112084	27.89%	2.377%
14	10.133	1207	1215	1227	rBV	909813	1665729	41.78%	3.560%
15	10.504	1270	1278	1289	rBV	1012676	1704436	42.75%	3.643%
16	10.645	1295	1302	1322	rBV	797286	1660460	41.65%	3.549%
17	11.780	1491	1495	1502	rVB5	6670	12606	0.32%	0.027%
18	12.122	1547	1553	1561	rBV2	11867	24589	0.62%	0.053%
19	13.769	1827	1833	1848	rBV	1612170	2303074	57.77%	4.922%
20	14.051	1873	1881	1894	rBV	1912373	2893732	72.58%	6.185%
21	14.357	1926	1933	1949	rBV	1466853	2142794	53.75%	4.580%
22	14.580	1965	1971	1989	rBV	327296	819506	20.55%	1.751%
23	15.351	2095	2102	2112	rBV	2370138	3435413	86.17%	7.342%
24	15.480	2117	2124	2138	rVV	599656	915662	22.97%	1.957%
25	15.592	2139	2143	2150	rVV4	15983	34415	0.86%	0.074%
26	16.598	2309	2314	2317	rBV4	4136	6497	0.16%	0.014%
27	16.886	2361	2363	2366	rBV4	4033	5143	0.13%	0.011%
28	17.098	2393	2399	2410	rBV	1634449	2290991	57.46%	4.896%
29	17.198	2410	2416	2437	rVB	2424030	3591102	90.07%	7.675%
30	17.657	2489	2494	2498	rBV5	4120	7662	0.19%	0.016%
31	19.056	2727	2732	2737	rBV4	27857	47150	1.18%	0.101%
32	19.127	2740	2744	2749	rBV	27380	42075	1.06%	0.090%
33	19.403	2789	2791	2793	rBV3	6846	5821	0.15%	0.012%
34	19.492	2800	2806	2816	rBV	2875974	3986927	100.00%	8.521%
35	21.321	3112	3117	3127	rBV	1345529	2219397	55.67%	4.743%
36	24.062	3575	3583	3595	rBV	1551401	3718958	93.28%	7.948%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048309.D
Acq On : 30 Oct 2024 05:50
Operator : RC/JU
Sample : PB164514BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK514

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	24.262	3609	3617	3633	rVB	914621	2395928	60.09%	5.121%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 46789397

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048309.D
Acq On : 30 Oct 2024 05:50
Operator : RC/JU
Sample : PB164514BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK514

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

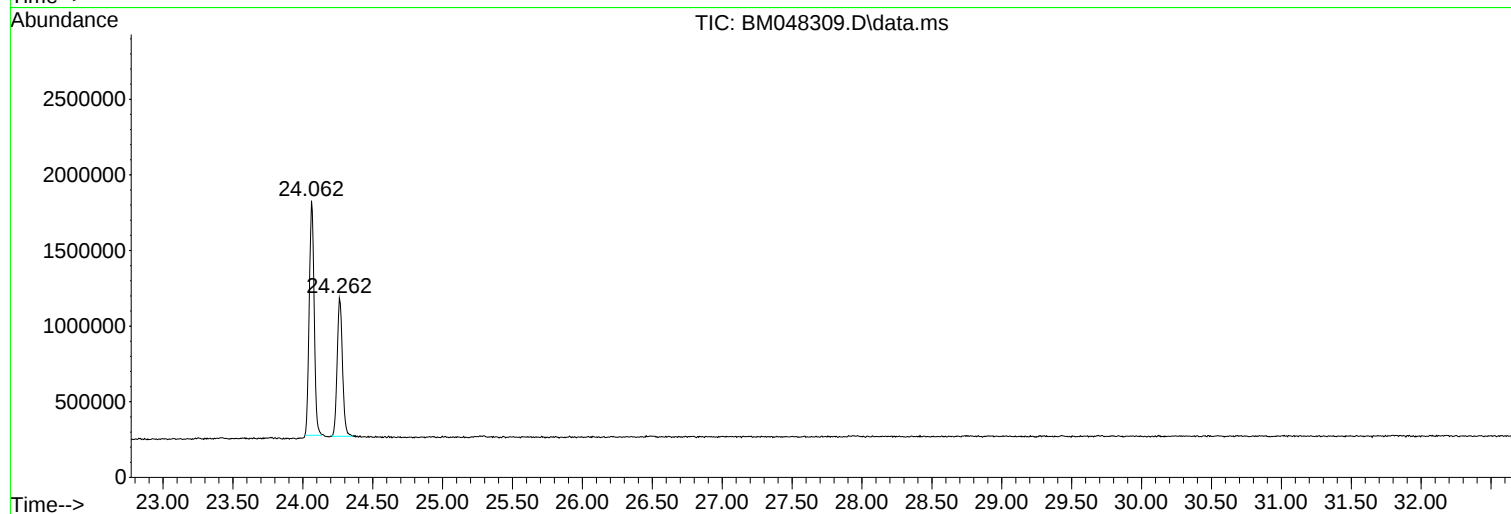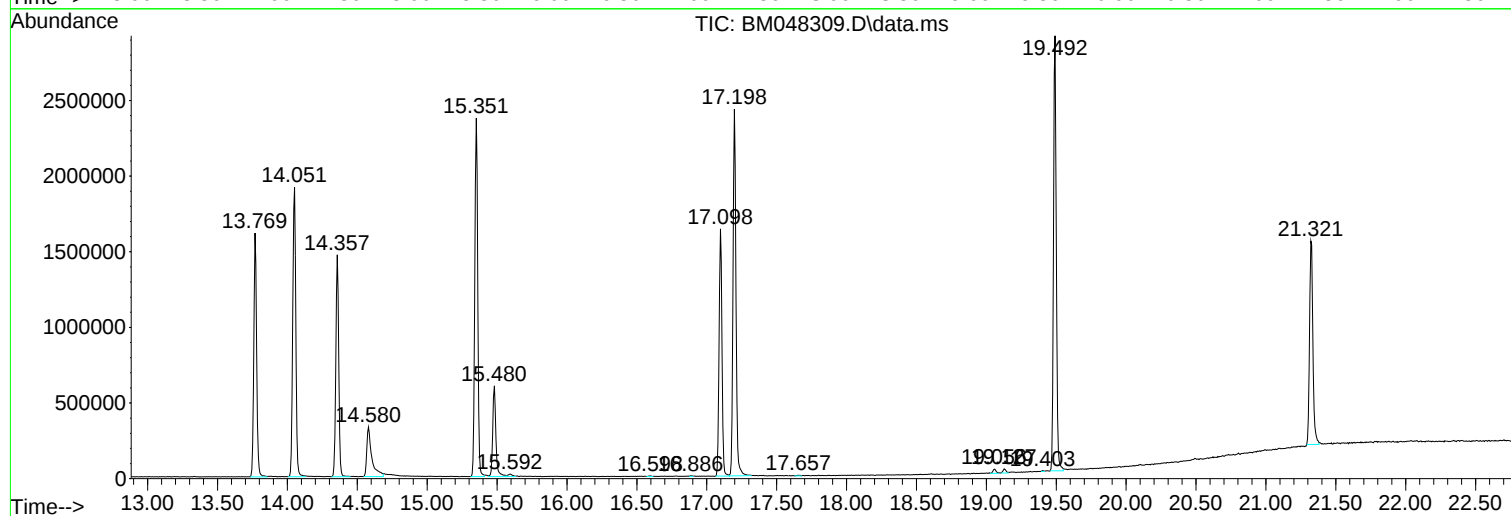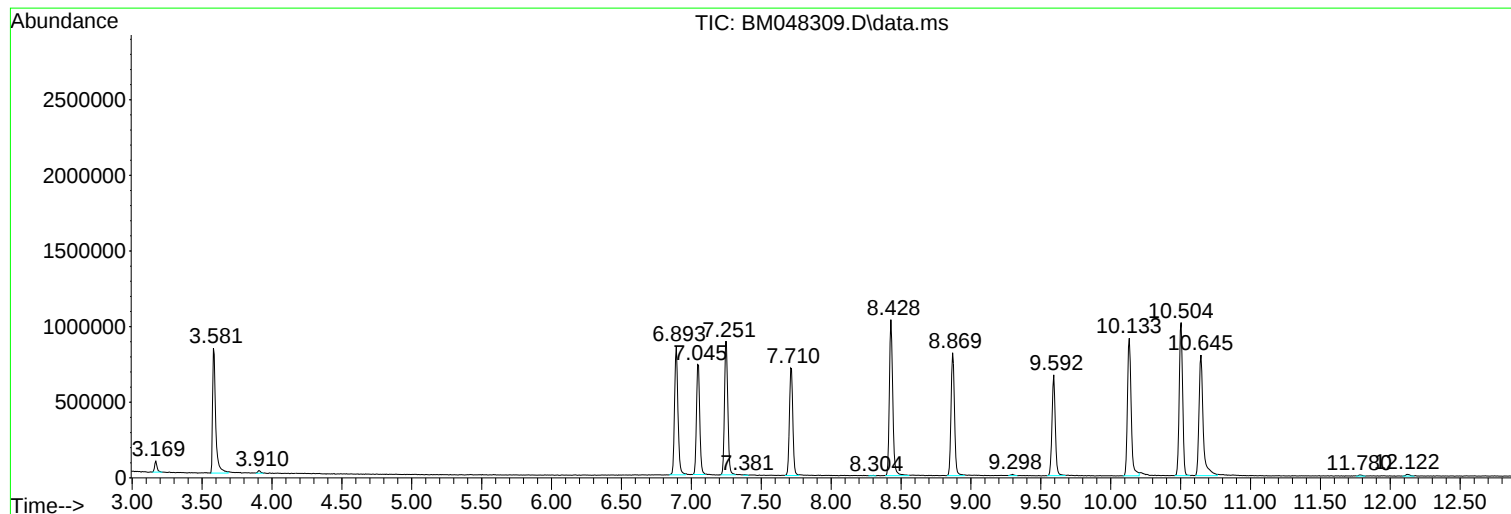

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048309.D
Acq On : 30 Oct 2024 05:50
Operator : RC/JU
Sample : PB164514BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK514

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048309.D
Acq On : 30 Oct 2024 05:50
Operator : RC/JU
Sample : PB164514BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK514

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc