

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048311.D
 Acq On : 30 Oct 2024 07:09
 Operator : RC/JU
 Sample : P4534-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	41	rVB	56350	72648	1.37%	0.145%
2	3.593	100	103	116	rBV	89271	161133	3.05%	0.322%
3	3.904	153	156	160	rVB2	10844	13024	0.25%	0.026%
4	4.846	314	316	319	rVB3	6112	5475	0.10%	0.011%
5	6.892	655	664	675	rVB	221810	391206	7.40%	0.782%
6	7.045	684	690	701	rBV	838049	1366844	25.84%	2.733%
7	7.251	718	725	734	rBV	870618	1461762	27.63%	2.923%
8	7.334	737	739	748	rVB6	7248	10446	0.20%	0.021%
9	7.716	796	804	813	rBV	644580	1073218	20.29%	2.146%
10	8.428	919	925	940	rBV	725353	1227460	23.20%	2.454%
11	8.869	992	1000	1010	rBV	983085	1624429	30.71%	3.248%
12	9.292	1066	1072	1077	rBV2	16250	26760	0.51%	0.054%
13	9.592	1115	1123	1136	rBV	798554	1351585	25.55%	2.703%
14	10.133	1207	1215	1236	rBV	1107276	2010881	38.01%	4.021%
15	10.504	1270	1278	1293	rVB	906787	1574554	29.77%	3.148%
16	10.645	1293	1302	1323	rBV	668309	1407261	26.60%	2.814%
17	11.339	1414	1420	1421	rBV4	4566	5446	0.10%	0.011%
18	11.786	1488	1496	1504	rVB4	12421	23402	0.44%	0.047%
19	12.116	1546	1552	1558	rBV3	13394	28573	0.54%	0.057%
20	13.327	1753	1758	1763	rBV7	3381	5788	0.11%	0.012%
21	13.768	1826	1833	1848	rBV	2042855	3018228	57.06%	6.035%
22	14.051	1874	1881	1899	rBV	2405393	3570815	67.50%	7.140%
23	14.357	1926	1933	1943	rBV	1359520	1988627	37.59%	3.976%
24	14.598	1968	1974	1990	rBV4	57164	195241	3.69%	0.390%
25	15.351	2093	2102	2114	rBV	3039691	4416707	83.49%	8.832%
26	15.480	2117	2124	2137	rVV	897560	1369716	25.89%	2.739%
27	15.592	2139	2143	2154	rVB7	17105	35813	0.68%	0.072%
28	15.921	2194	2199	2201	rBV5	4200	6893	0.13%	0.014%
29	16.068	2219	2224	2225	rBV4	8695	12673	0.24%	0.025%
30	16.133	2232	2235	2238	rVB5	4246	5859	0.11%	0.012%
31	16.592	2310	2313	2319	rBV6	4829	7885	0.15%	0.016%
32	16.780	2342	2345	2348	rVB5	5319	5924	0.11%	0.012%
33	17.098	2392	2399	2409	rBV	1511036	2100515	39.71%	4.200%
34	17.198	2410	2416	2434	rVV	3330430	4716706	89.17%	9.431%
35	17.774	2509	2514	2517	rBV7	5329	10193	0.19%	0.020%
36	17.998	2548	2552	2558	rBV6	21817	39190	0.74%	0.078%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048311.D
Acq On : 30 Oct 2024 07:09
Operator : RC/JU
Sample : P4534-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L62

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	18.068	2561	2564	2567	rVB3	6768	7981	0.15%	0.016%
38	19.056	2727	2732	2737	rBV3	43599	59797	1.13%	0.120%
39	19.127	2740	2744	2748	rVV	37323	49024	0.93%	0.098%
40	19.280	2766	2770	2773	rBV5	21305	27564	0.52%	0.055%
41	19.492	2800	2806	2821	rBV	3869936	5289829	100.00%	10.577%
42	21.321	3112	3117	3130	rBV2	1273512	2043739	38.64%	4.087%
43	24.068	3575	3584	3598	rVB	2027678	5014818	94.80%	10.027%
44	24.268	3609	3618	3634	rVB	832130	2175157	41.12%	4.349%




Sum of corrected areas: 50010789

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048311.D
Acq On : 30 Oct 2024 07:09
Operator : RC/JU
Sample : P4534-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

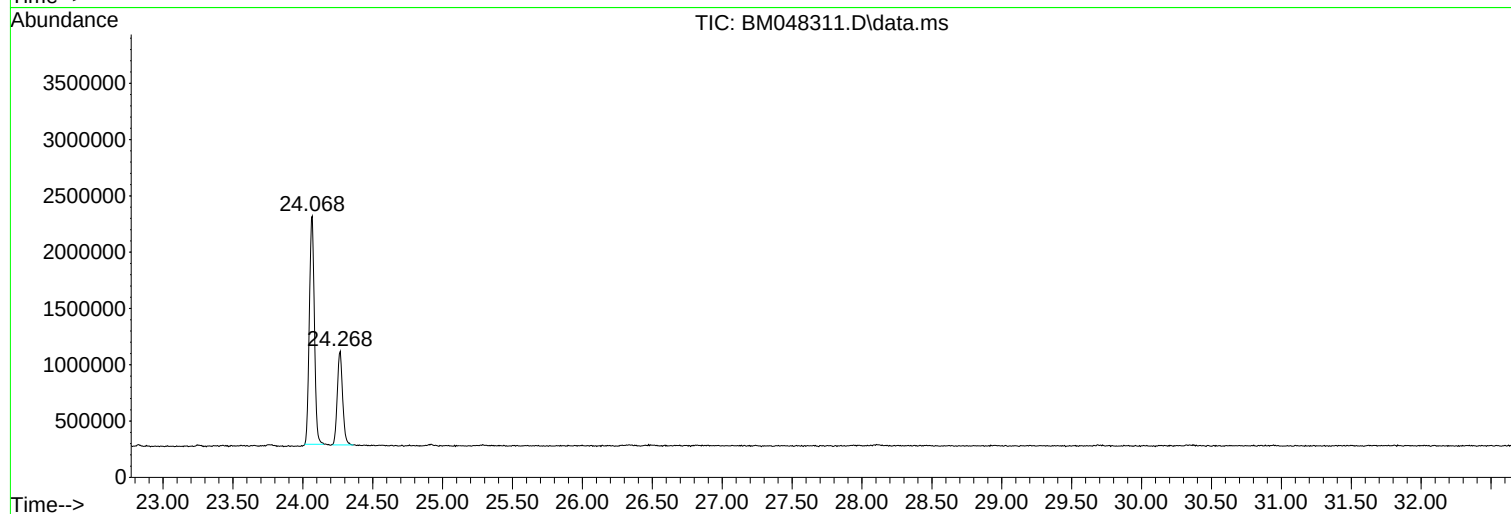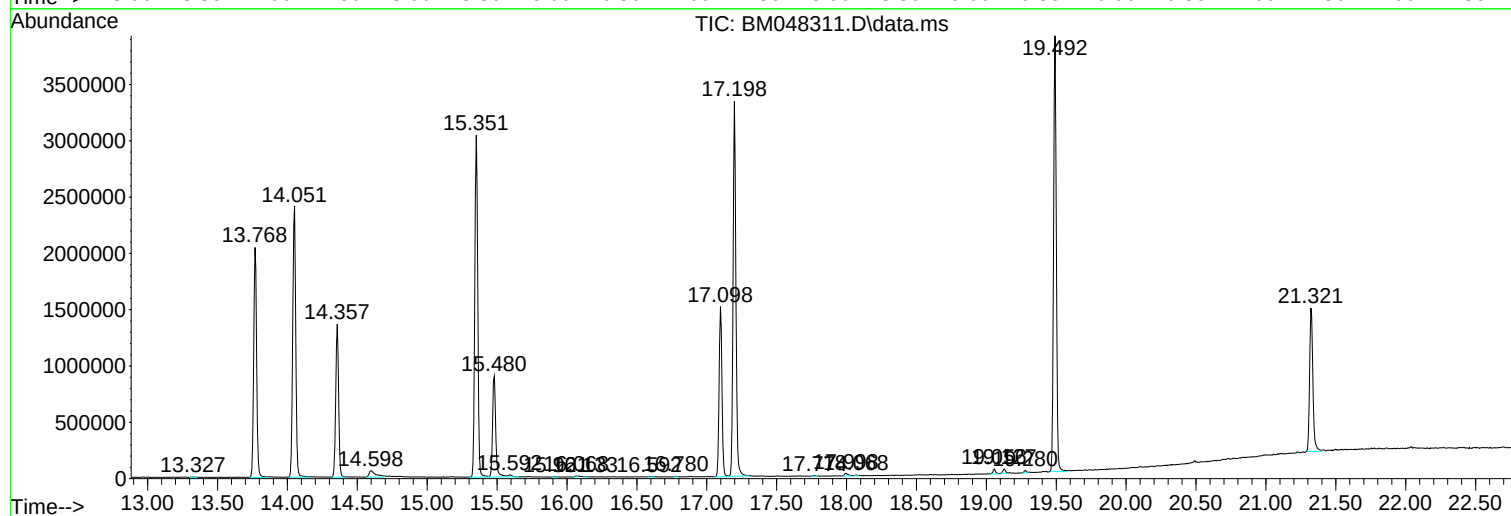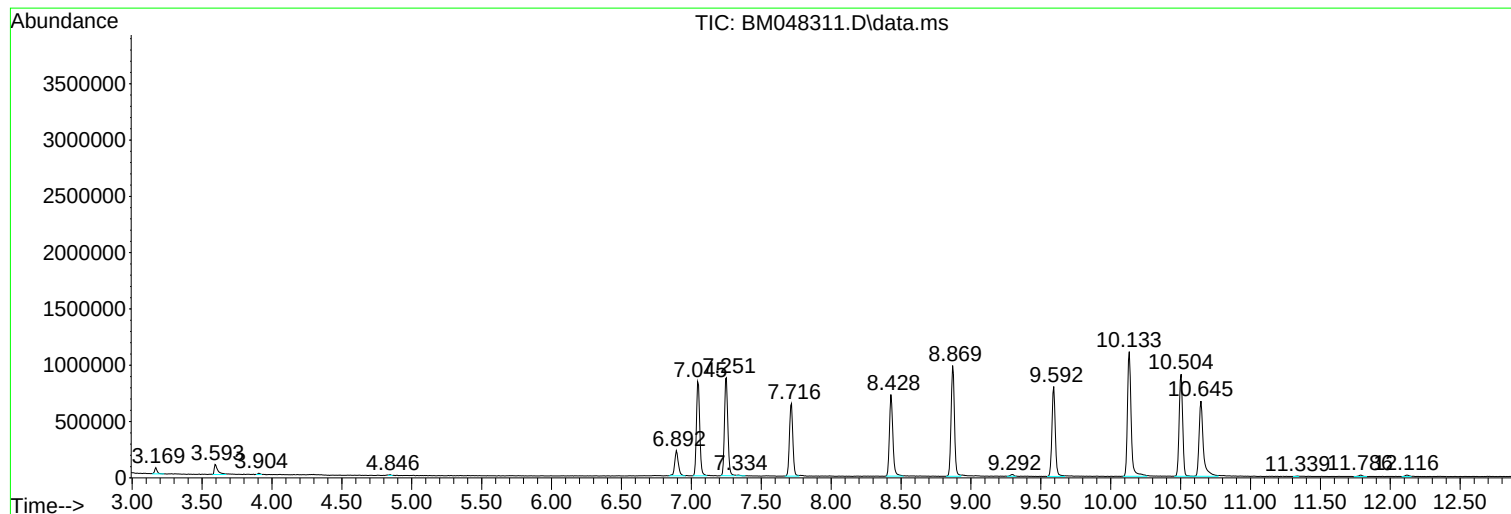

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048311.D
Acq On : 30 Oct 2024 07:09
Operator : RC/JU
Sample : P4534-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048311.D
Acq On : 30 Oct 2024 07:09
Operator : RC/JU
Sample : P4534-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc