

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048318.D
 Acq On : 30 Oct 2024 11:44
 Operator : RC/JU
 Sample : PB164464BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK464

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	39	rVB	59581	81787	2.48%	0.196%
2	3.546	92	95	98	rBV5	4391	6492	0.20%	0.016%
3	3.581	98	101	118	rVV	669467	1046633	31.78%	2.511%
4	3.910	152	157	164	rBV	63276	95796	2.91%	0.230%
5	4.910	325	327	332	rVB5	3079	3366	0.10%	0.008%
6	5.363	401	404	407	rBV4	2766	4067	0.12%	0.010%
7	6.893	656	664	678	rBV	683945	1160655	35.24%	2.785%
8	7.046	683	690	705	rVB	606499	982793	29.84%	2.358%
9	7.246	718	724	741	rBV	737468	1233873	37.46%	2.960%
10	7.710	797	803	814	rBV	749713	1252802	38.04%	3.006%
11	8.122	870	873	877	rBV6	2240	3392	0.10%	0.008%
12	8.240	890	893	897	rBV6	2228	3867	0.12%	0.009%
13	8.428	918	925	938	rBV	850909	1452384	44.10%	3.485%
14	8.869	991	1000	1012	rBV	683835	1148516	34.87%	2.755%
15	9.245	1059	1064	1066	rBV6	2690	4241	0.13%	0.010%
16	9.298	1069	1073	1081	rVB6	9394	14076	0.43%	0.034%
17	9.592	1116	1123	1135	rBV	537684	940011	28.54%	2.255%
18	9.728	1143	1146	1149	rVB5	4134	5273	0.16%	0.013%
19	10.134	1208	1215	1227	rBV	756978	1379849	41.90%	3.310%
20	10.504	1270	1278	1285	rVV	1045573	1802719	54.74%	4.325%
21	10.645	1295	1302	1325	rBV	649918	1426525	43.31%	3.422%
22	11.439	1432	1437	1442	rBV8	2395	5064	0.15%	0.012%
23	11.786	1493	1496	1502	rVB5	5705	7630	0.23%	0.018%
24	12.128	1548	1554	1558	rBV4	10309	22974	0.70%	0.055%
25	12.245	1573	1574	1582	rVB6	1927	4334	0.13%	0.010%
26	13.769	1826	1833	1850	rBV	1354059	1956188	59.40%	4.693%
27	14.051	1873	1881	1897	rBV	1545502	2423335	73.58%	5.814%
28	14.280	1916	1920	1923	rBV6	2036	3415	0.10%	0.008%
29	14.357	1925	1933	1943	rBV	1528209	2249532	68.30%	5.397%
30	14.586	1961	1972	1987	rBV	231911	631511	19.17%	1.515%
31	15.351	2095	2102	2118	rBV	1974522	2910116	88.36%	6.982%
32	15.480	2118	2124	2139	rVV	426604	703599	21.36%	1.688%
33	15.586	2139	2142	2149	rVB6	10815	19887	0.60%	0.048%
34	15.868	2185	2190	2192	rBV5	2784	3854	0.12%	0.009%
35	15.921	2192	2199	2203	rVB9	2242	5681	0.17%	0.014%
36	16.598	2308	2314	2317	rBV5	4282	8362	0.25%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048318.D
 Acq On : 30 Oct 2024 11:44
 Operator : RC/JU
 Sample : PB164464BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK464

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

37	16.716	2328	2334	2336	rBV6	2024	3595	0.11%	0.009%
38	16.886	2358	2363	2365	rBV3	3950	5595	0.17%	0.013%
39	17.098	2393	2399	2410	rBV	1650601	2417530	73.40%	5.800%
40	17.198	2410	2416	2431	rVV	2015065	2992724	90.87%	7.180%
41	17.298	2431	2433	2437	rVB5	4954	5631	0.17%	0.014%
42	17.815	2518	2521	2523	rBV3	3680	4153	0.13%	0.010%
43	18.609	2652	2656	2657	rBV3	4849	6068	0.18%	0.015%
44	19.057	2728	2732	2738	rBV4	24960	38634	1.17%	0.093%
45	19.133	2741	2745	2749	rVV	18764	27511	0.84%	0.066%
46	19.492	2800	2806	2818	rBV	2393824	3293514	100.00%	7.902%
47	21.327	3112	3118	3132	rBV	1421492	2328174	70.69%	5.586%
48	24.062	3575	3583	3597	rVB	1243833	3041580	92.35%	7.297%
49	24.268	3610	3618	3633	rVB	953041	2511957	76.27%	6.027%


Sum of corrected areas: 41681265

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048318.D
Acq On : 30 Oct 2024 11:44
Operator : RC/JU
Sample : PB164464BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK464

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

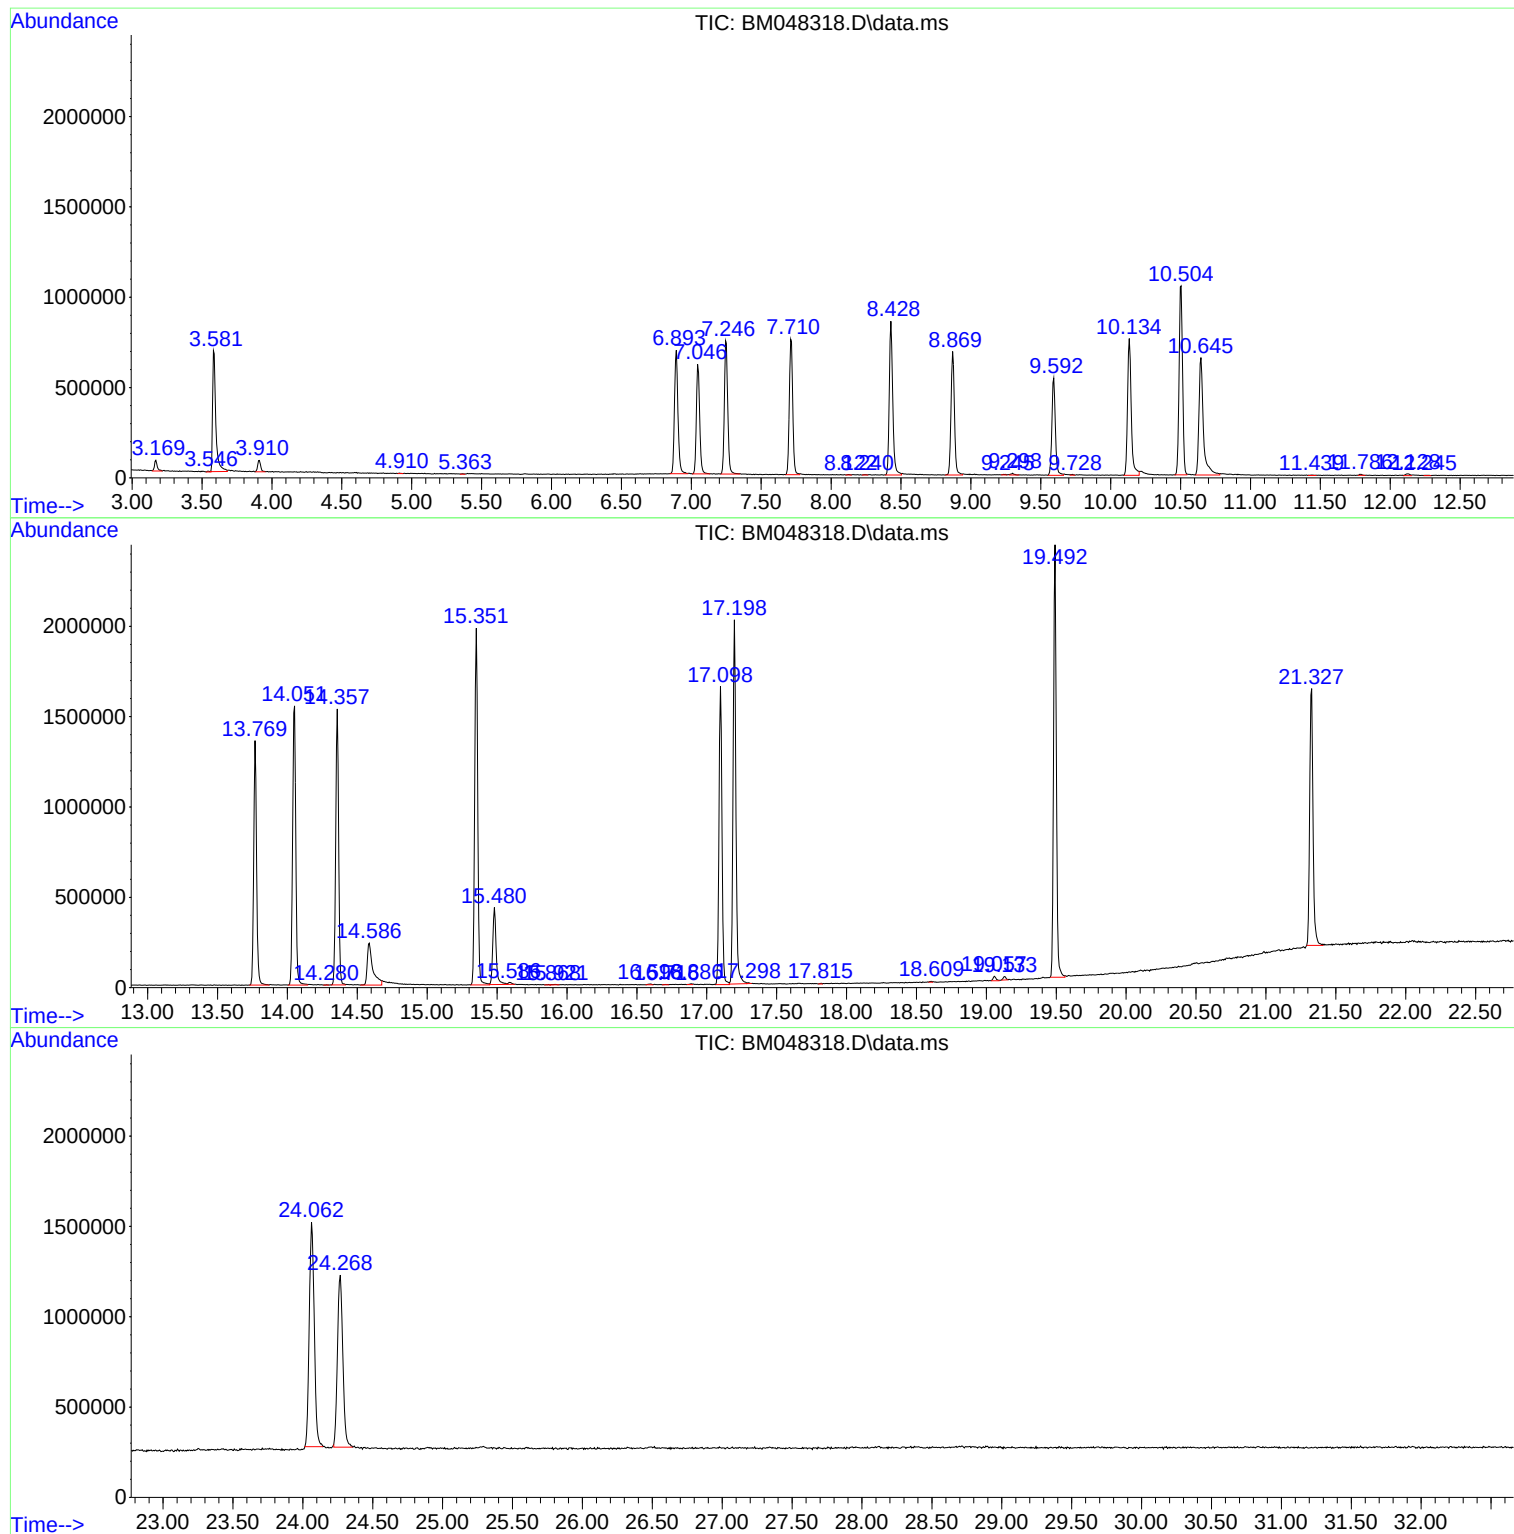

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048318.D
Acq On : 30 Oct 2024 11:44
Operator : RC/JU
Sample : PB164464BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK464

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048318.D
Acq On : 30 Oct 2024 11:44
Operator : RC/JU
Sample : PB164464BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK464

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------