

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048319.D
 Acq On : 30 Oct 2024 12:24
 Operator : RC/JU
 Sample : PB164448BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK448

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048319.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.170	27	31	39	rVB	70356	90438	2.42%	0.193%
2	3.581	97	101	122	rBV	839225	1265346	33.86%	2.696%
3	3.911	153	157	160	rVB4	13467	18845	0.50%	0.040%
4	6.734	634	637	640	rBV5	2848	4624	0.12%	0.010%
5	6.893	654	664	680	rBV	842484	1421649	38.04%	3.029%
6	7.046	684	690	701	rVV	725249	1177350	31.50%	2.509%
7	7.246	718	724	738	rBV	900284	1475911	39.49%	3.145%
8	7.710	796	803	812	rBV	782627	1305196	34.93%	2.781%
9	8.428	918	925	943	rVV	1031899	1760564	47.11%	3.751%
10	8.569	946	949	954	rVB6	2603	5102	0.14%	0.011%
11	8.869	992	1000	1012	rBV	834003	1386013	37.09%	2.953%
12	9.293	1069	1072	1079	rVB4	10526	16617	0.44%	0.035%
13	9.593	1116	1123	1141	rBV	653174	1140254	30.51%	2.430%
14	10.134	1207	1215	1227	rBV	923063	1675464	44.83%	3.570%
15	10.504	1265	1278	1287	rBV	1101271	1902923	50.92%	4.055%
16	10.646	1294	1302	1323	rBV	816253	1724037	46.13%	3.673%
17	11.787	1489	1496	1502	rBV4	10979	17650	0.47%	0.038%
18	12.122	1547	1553	1558	rBV5	12045	21038	0.56%	0.045%
19	13.769	1827	1833	1849	rBV	1647533	2310006	61.81%	4.922%
20	13.881	1849	1852	1858	rVB8	3622	6453	0.17%	0.014%
21	14.051	1874	1881	1891	rVV	1855860	2875370	76.94%	6.127%
22	14.357	1926	1933	1945	rBV	1571450	2377926	63.63%	5.067%
23	14.581	1964	1971	1995	rBV	300452	805896	21.56%	1.717%
24	15.351	2095	2102	2113	rBV	2342590	3406691	91.16%	7.259%
25	15.481	2118	2124	2137	rVV	543831	834421	22.33%	1.778%
26	15.592	2140	2143	2149	rVB5	12418	21370	0.57%	0.046%
27	16.598	2310	2314	2316	rBV5	4053	4133	0.11%	0.009%
28	16.886	2361	2363	2366	rBV4	4862	6124	0.16%	0.013%
29	17.098	2393	2399	2409	rBV	1762974	2465264	65.97%	5.253%
30	17.198	2410	2416	2434	rVV	2399002	3457506	92.52%	7.367%
31	17.339	2438	2440	2444	rVB5	4094	3782	0.10%	0.008%
32	17.663	2490	2495	2497	rBV5	5387	6945	0.19%	0.015%
33	19.057	2728	2732	2736	rBV2	23768	31997	0.86%	0.068%
34	19.127	2740	2744	2750	rBV	25653	36705	0.98%	0.078%
35	19.492	2800	2806	2818	rBV	2582863	3737134	100.00%	7.963%
36	21.321	3112	3117	3129	rBV	1391335	2296690	61.46%	4.894%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048319.D
Acq On : 30 Oct 2024 12:24
Operator : RC/JU
Sample : PB164448BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK448

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	24.062	3575	3583	3599	rVB	1413520	3378641	90.41%	7.199%
38	24.268	3610	3618	3635	rVB	947137	2459718	65.82%	5.241%




Sum of corrected areas: 46931793

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048319.D
Acq On : 30 Oct 2024 12:24
Operator : RC/JU
Sample : PB164448BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

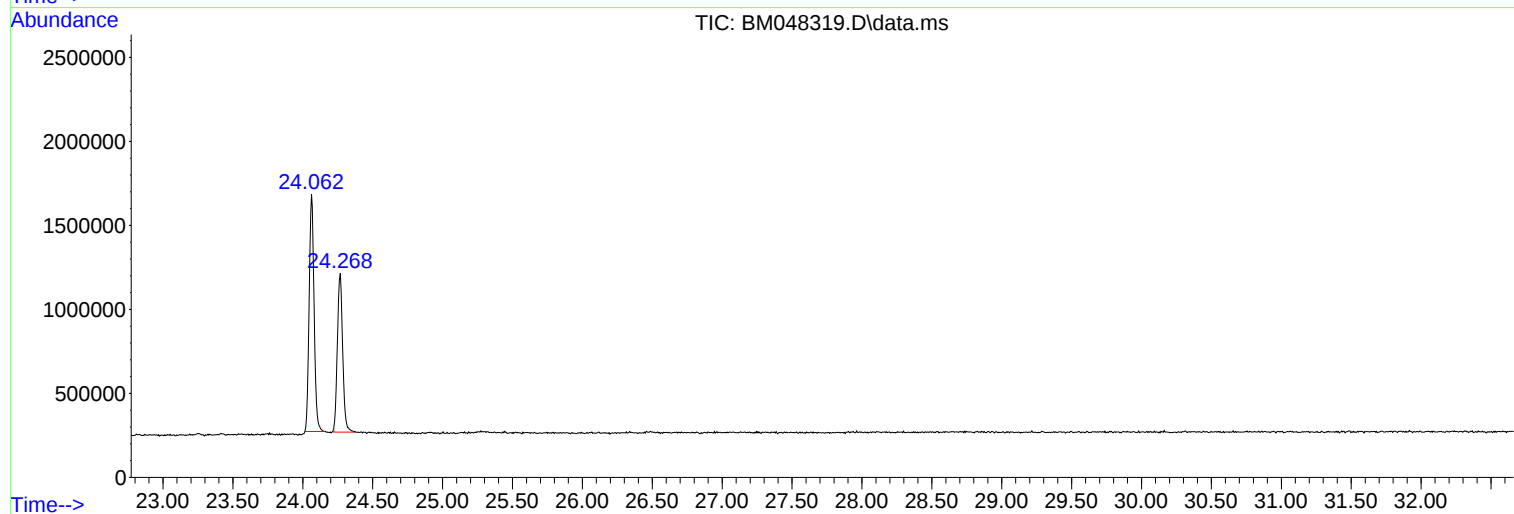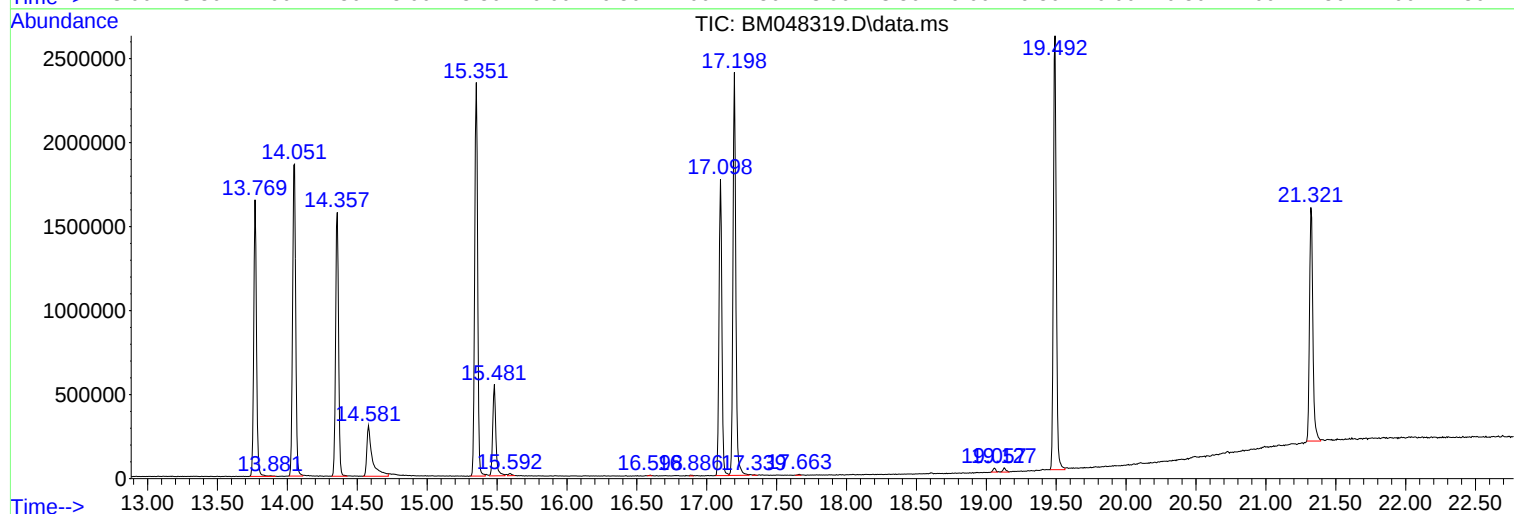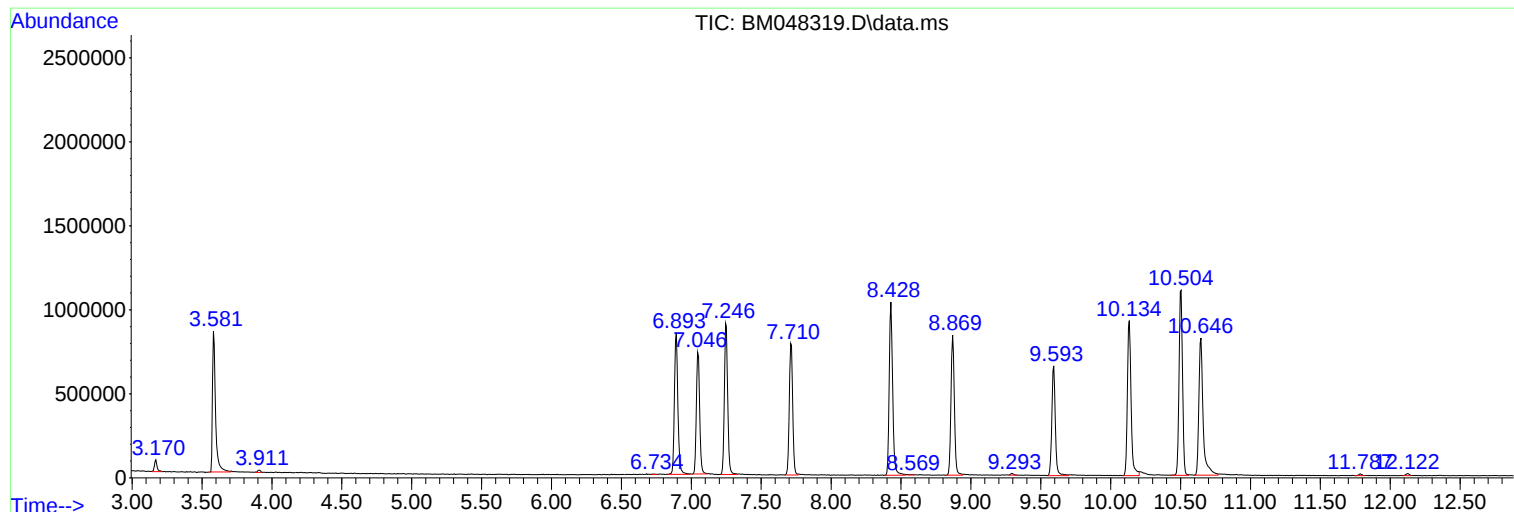

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048319.D
Acq On : 30 Oct 2024 12:24
Operator : RC/JU
Sample : PB164448BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048319.D
Acq On : 30 Oct 2024 12:24
Operator : RC/JU
Sample : PB164448BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------