

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048324.D
 Acq On : 30 Oct 2024 15:41
 Operator : RC/JU
 Sample : P4534-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1LB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	36	rVB	59215	74301	1.42%	0.141%
2	3.593	100	103	114	rBV	152293	250910	4.79%	0.476%
3	3.910	152	157	162	rBV3	13618	21811	0.42%	0.041%
4	4.822	309	312	314	rBV3	4144	5632	0.11%	0.011%
5	6.722	629	635	636	rBV5	2936	5816	0.11%	0.011%
6	6.893	653	664	676	rBV	241107	429649	8.20%	0.815%
7	7.045	683	690	700	rBV	891337	1427422	27.25%	2.706%
8	7.245	718	724	735	rBV	939617	1540419	29.41%	2.921%
9	7.340	737	740	743	rVB5	6609	8941	0.17%	0.017%
10	7.710	796	803	813	rBV	838008	1408583	26.89%	2.671%
11	8.428	919	925	941	rBV	778641	1308421	24.98%	2.481%
12	8.869	991	1000	1009	rBV	1016999	1685483	32.18%	3.196%
13	9.298	1065	1073	1077	rVB2	21331	37467	0.72%	0.071%
14	9.592	1116	1123	1137	rBV	784767	1382746	26.40%	2.622%
15	10.134	1207	1215	1240	rBV	1078605	2125256	40.58%	4.030%
16	10.498	1270	1277	1288	rBV	1208979	2055360	39.24%	3.897%
17	10.657	1296	1304	1323	rBV	113568	323460	6.18%	0.613%
18	10.775	1323	1324	1331	rVB7	3419	5311	0.10%	0.010%
19	11.786	1490	1496	1502	rBV2	18129	29956	0.57%	0.057%
20	12.116	1547	1552	1558	rBV5	12078	23530	0.45%	0.045%
21	12.351	1588	1592	1597	rVB2	4188	6713	0.13%	0.013%
22	12.969	1692	1697	1702	rBV7	3929	8098	0.15%	0.015%
23	13.769	1827	1833	1849	rBV	2196048	3123235	59.63%	5.922%
24	14.051	1873	1881	1893	rBV	2324620	3541781	67.62%	6.715%
25	14.357	1926	1933	1946	rBV	1749836	2588844	49.43%	4.908%
26	14.598	1968	1974	1986	rBV2	62025	184807	3.53%	0.350%
27	15.163	2065	2070	2072	rBV4	5401	8518	0.16%	0.016%
28	15.351	2095	2102	2116	rBV	3139751	4550559	86.88%	8.628%
29	15.474	2118	2123	2140	rVV	877753	1390836	26.55%	2.637%
30	15.592	2140	2143	2151	rVB5	17601	31139	0.59%	0.059%
31	16.068	2220	2224	2233	rBV4	9389	25384	0.48%	0.048%
32	16.133	2233	2235	2239	rVB5	4491	5483	0.10%	0.010%
33	16.580	2307	2311	2319	rVV6	21396	42173	0.81%	0.080%
34	16.704	2327	2332	2338	rVB3	22042	33282	0.64%	0.063%
35	16.780	2342	2345	2349	rVB5	6135	5819	0.11%	0.011%
36	17.033	2384	2388	2391	rVB6	4004	5762	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048324.D
 Acq On : 30 Oct 2024 15:41
 Operator : RC/JU
 Sample : P4534-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1LB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

37	17.098	2391	2399	2409	rBV	1923148	2691159	51.38%	5.102%
38	17.198	2409	2416	2430	rVV	3345830	4826582	92.15%	9.151%
39	17.662	2492	2495	2497	rBV4	4930	6344	0.12%	0.012%
40	17.686	2497	2499	2503	rVB4	3850	5547	0.11%	0.011%
41	17.998	2548	2552	2558	rBV8	11538	18661	0.36%	0.035%
42	18.068	2561	2564	2567	rVB3	7425	9258	0.18%	0.018%
43	18.274	2595	2599	2607	rBV	19632	29427	0.56%	0.056%
44	18.515	2638	2640	2645	rBV6	3281	5728	0.11%	0.011%
45	18.604	2653	2655	2659	rVB5	6245	7926	0.15%	0.015%
46	19.056	2727	2732	2737	rBV2	40244	60478	1.15%	0.115%
47	19.127	2740	2744	2750	rBV	36693	56416	1.08%	0.107%
48	19.280	2766	2770	2773	rBV5	14937	25236	0.48%	0.048%
49	19.492	2800	2806	2821	rBV	3874347	5237613	100.00%	9.931%
50	21.321	3112	3117	3131	rBV	1613343	2588289	49.42%	4.907%
51	24.068	3575	3584	3596	rBV	1906246	4811459	91.86%	9.123%
52	24.268	3610	3618	3631	rVB	1033916	2659328	50.77%	5.042%


Sum of corrected areas: 52742358

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048324.D
Acq On : 30 Oct 2024 15:41
Operator : RC/JU
Sample : P4534-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1LB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

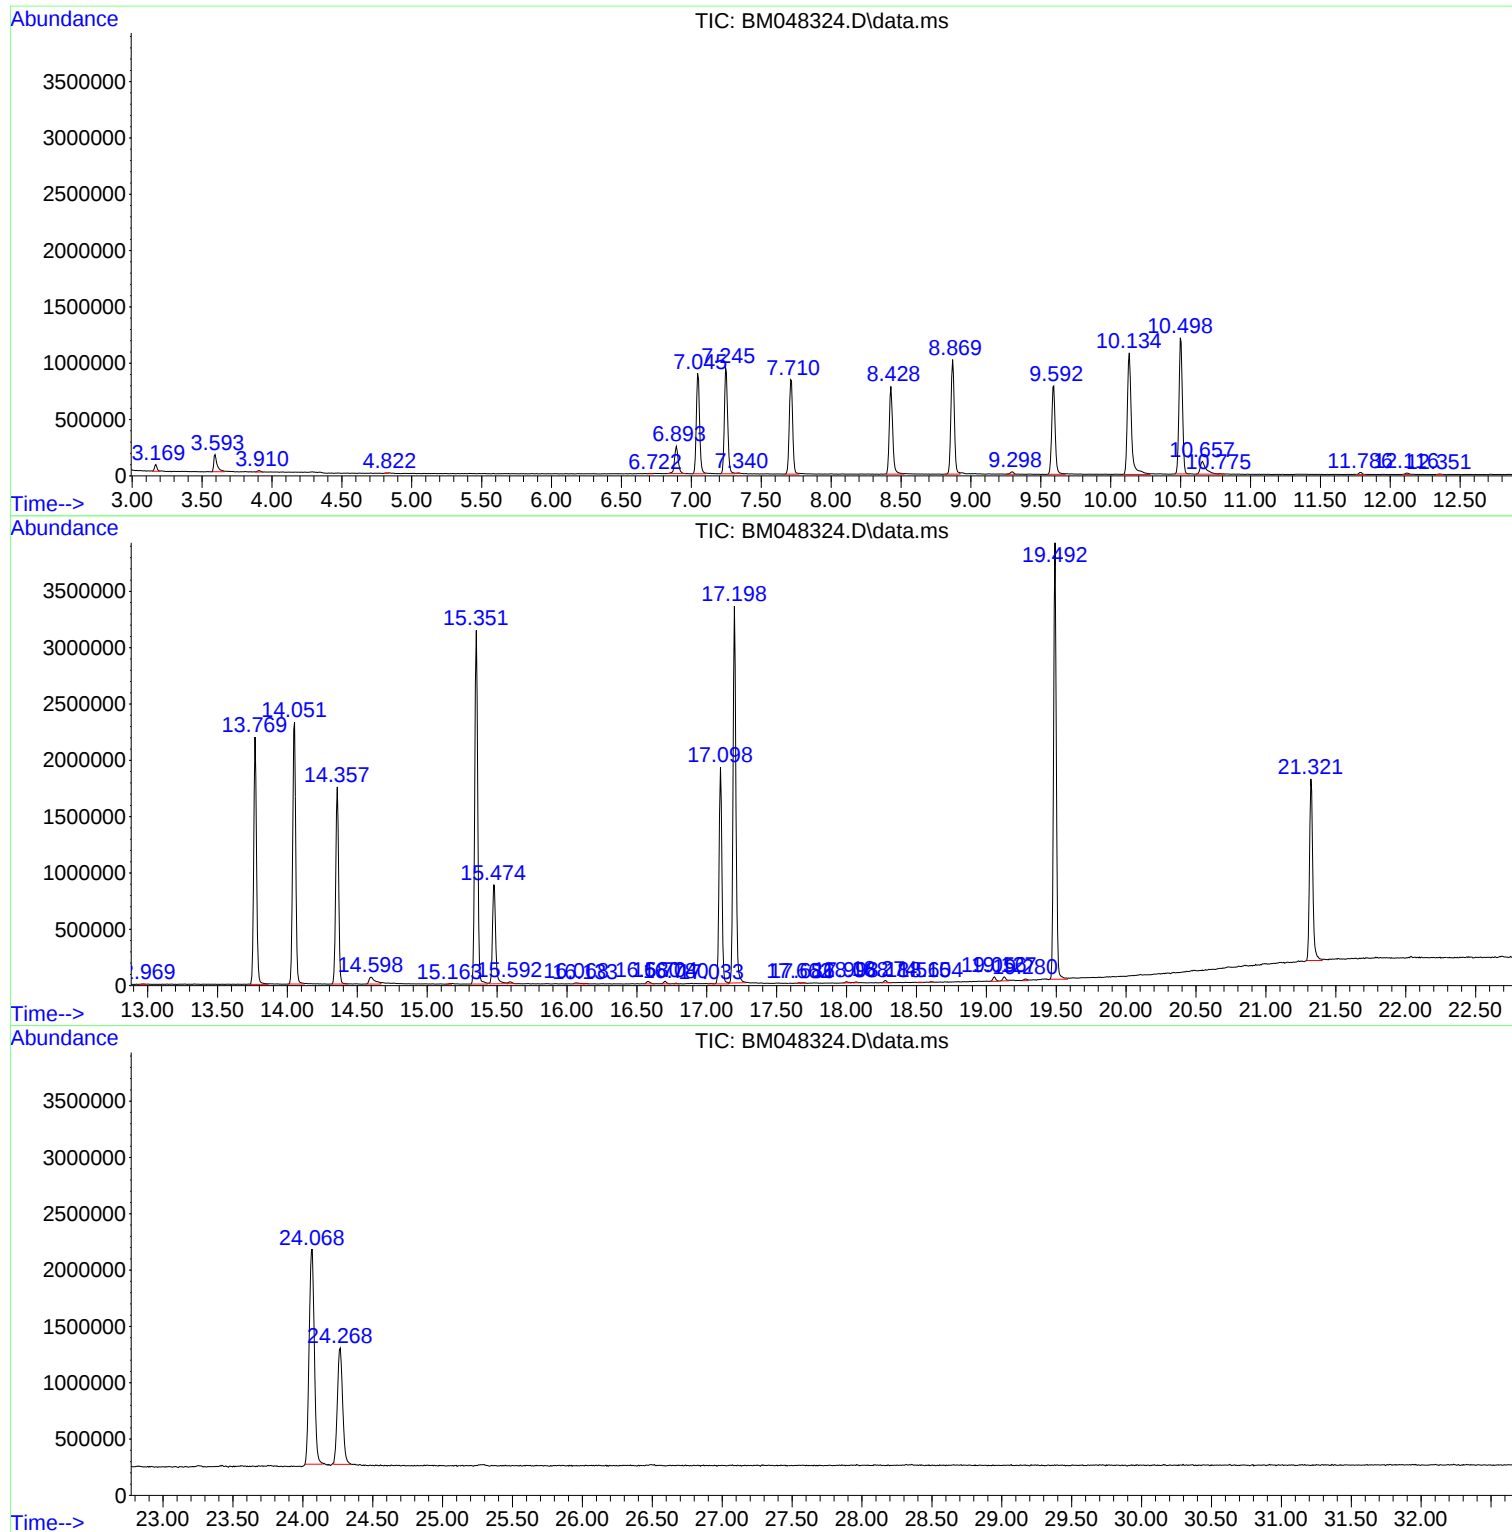

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048324.D
Acq On : 30 Oct 2024 15:41
Operator : RC/JU
Sample : P4534-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1LB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048324.D
Acq On : 30 Oct 2024 15:41
Operator : RC/JU
Sample : P4534-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1LB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc