

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048336.D
 Acq On : 31 Oct 2024 00:13
 Operator : RC/JU
 Sample : P4534-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	39	rVB	56456	76568	1.36%	0.147%
2	3.593	99	103	117	rBV	166088	291068	5.16%	0.560%
3	3.910	154	157	160	rVB3	13384	15183	0.27%	0.029%
4	6.893	658	664	673	rVB	223702	381622	6.76%	0.734%
5	7.045	684	690	700	rBV	820835	1287250	22.81%	2.475%
6	7.245	717	724	737	rBV	888989	1446521	25.63%	2.781%
7	7.710	794	803	812	rBV	782547	1271002	22.52%	2.444%
8	8.428	917	925	941	rBV	692082	1185764	21.01%	2.280%
9	8.534	941	943	949	rVB6	5574	8767	0.16%	0.017%
10	8.869	993	1000	1009	rBV	856196	1470324	26.06%	2.827%
11	9.298	1067	1073	1079	rVB2	19177	33112	0.59%	0.064%
12	9.586	1114	1122	1134	rBV	700144	1200779	21.28%	2.309%
13	10.128	1207	1214	1239	rBV	992386	1853315	32.84%	3.563%
14	10.498	1269	1277	1288	rBV	1083798	1806537	32.01%	3.473%
15	10.639	1294	1301	1321	rBV	728833	1565848	27.75%	3.011%
16	11.786	1492	1496	1502	rVB2	17565	31519	0.56%	0.061%
17	12.122	1548	1553	1559	rBV3	12492	22679	0.40%	0.044%
18	13.769	1826	1833	1846	rBV	1853539	2698293	47.82%	5.188%
19	14.045	1872	1880	1892	rBV2	2081515	3151559	55.85%	6.060%
20	14.357	1925	1933	1943	rBV	1500141	2284898	40.49%	4.393%
21	14.598	1968	1974	1988	rBV2	54355	180408	3.20%	0.347%
22	15.174	2065	2072	2076	rBV8	4557	10120	0.18%	0.019%
23	15.351	2094	2102	2111	rBV	2747307	4065206	72.04%	7.816%
24	15.474	2117	2123	2140	rBV	817840	1250964	22.17%	2.405%
25	15.592	2140	2143	2150	rVB6	16876	26706	0.47%	0.051%
26	15.721	2162	2165	2170	rVB7	3565	5840	0.10%	0.011%
27	16.068	2215	2224	2231	rBV8	6079	20337	0.36%	0.039%
28	16.592	2308	2313	2317	rBV4	8749	13562	0.24%	0.026%
29	16.880	2358	2362	2366	rVB7	5185	7278	0.13%	0.014%
30	17.098	2392	2399	2409	rBV	1846683	2522542	44.70%	4.850%
31	17.198	2409	2416	2435	rVV	3144421	4719970	83.64%	9.075%
32	17.662	2492	2495	2500	rVB7	6539	9033	0.16%	0.017%
33	17.992	2547	2551	2559	rBV3	29719	54078	0.96%	0.104%
34	18.068	2561	2564	2568	rVB4	5463	8190	0.15%	0.016%
35	18.492	2632	2636	2638	rBV5	5451	7493	0.13%	0.014%
36	19.056	2728	2732	2737	rBV3	38981	54197	0.96%	0.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048336.D
Acq On : 31 Oct 2024 00:13
Operator : RC/JU
Sample : P4534-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L63

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	19.127	2740	2744	2748	rBV	37788	53024	0.94%	0.102%
38	19.280	2766	2770	2773	rBV5	18933	24494	0.43%	0.047%
39	19.486	2799	2805	2821	rBV	3887144	5566403	98.64%	10.703%
40	21.321	3111	3117	3135	rBV	1711299	2728148	48.35%	5.245%
41	24.062	3574	3583	3596	rBV	2306603	5642996	100.00%	10.850%
42	24.262	3609	3617	3638	rVB	1132897	2956426	52.39%	5.684%




Sum of corrected areas: 52010023

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048336.D
Acq On : 31 Oct 2024 00:13
Operator : RC/JU
Sample : P4534-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

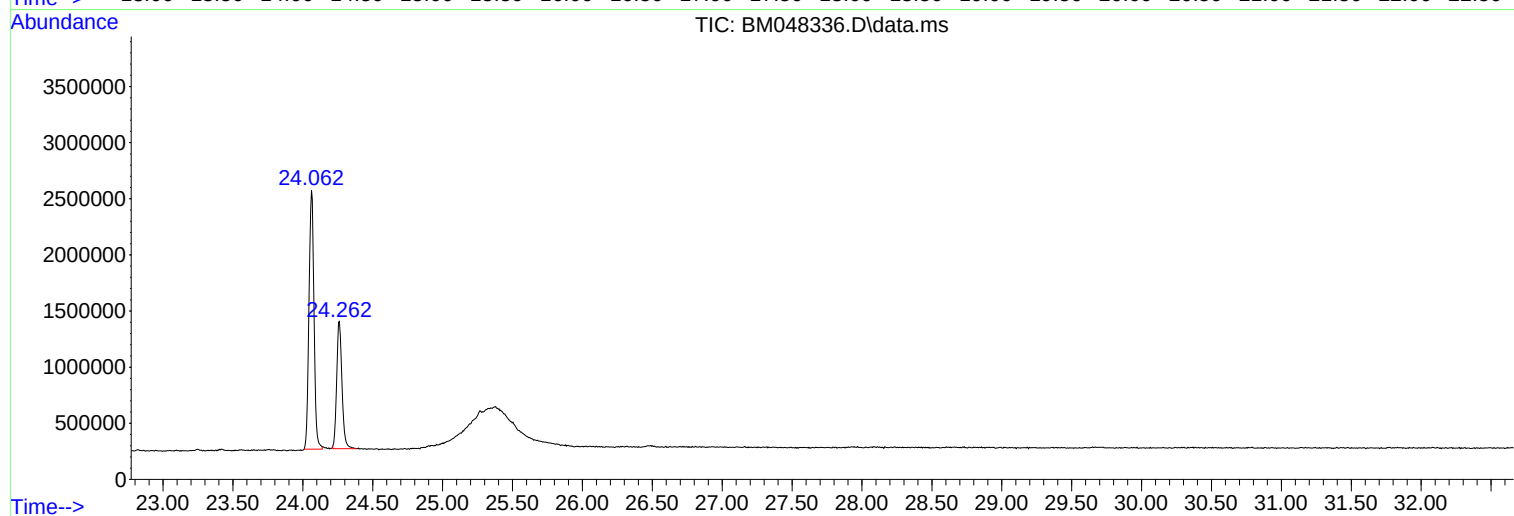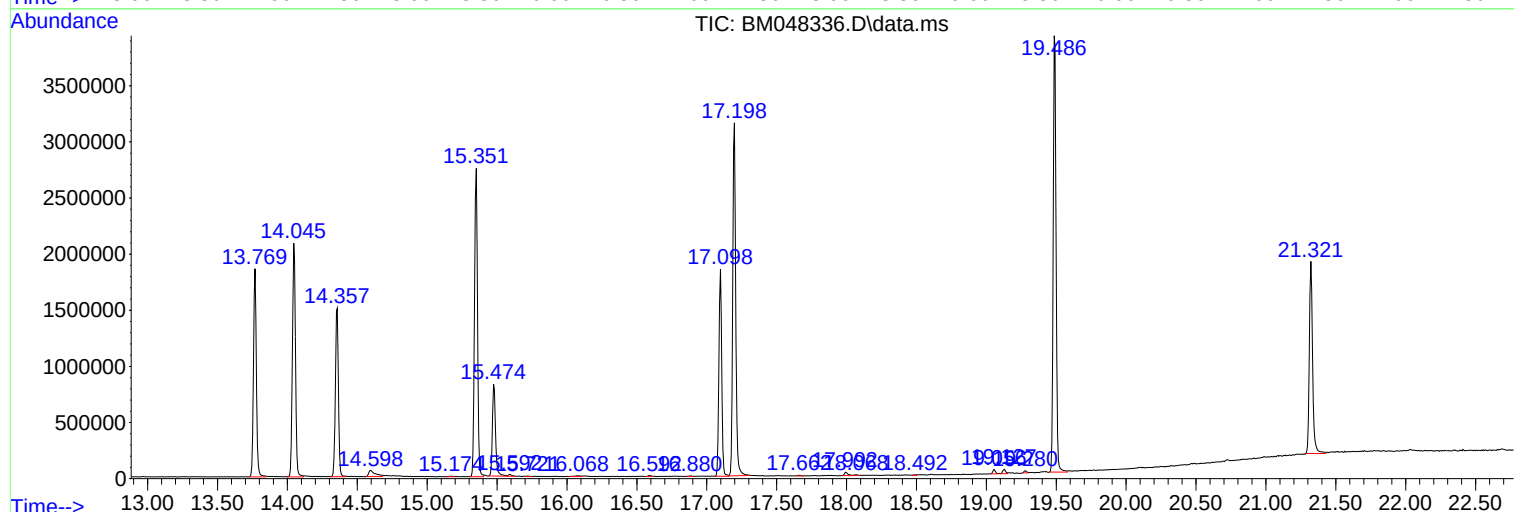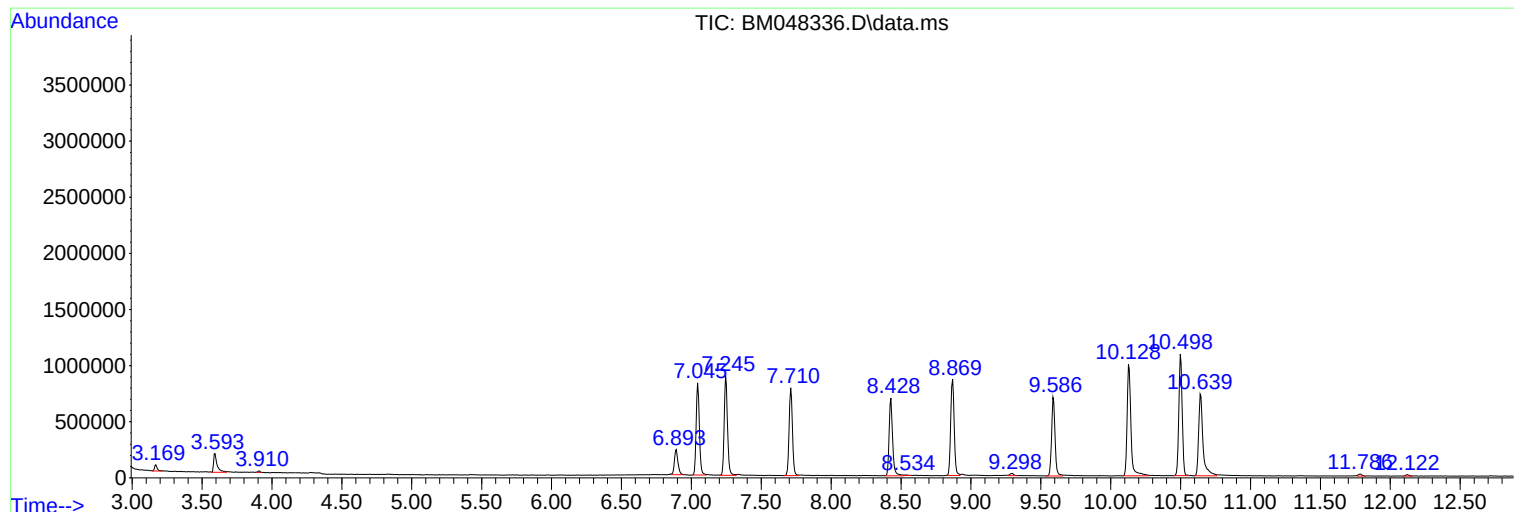

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048336.D
Acq On : 31 Oct 2024 00:13
Operator : RC/JU
Sample : P4534-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048336.D
Acq On : 31 Oct 2024 00:13
Operator : RC/JU
Sample : P4534-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc