

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048339.D
 Acq On : 31 Oct 2024 02:11
 Operator : RC/JU
 Sample : P4534-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.170	27	31	39	rVB	57711	77583	1.52%	0.140%
2	3.593	99	103	112	rBV	138723	242148	4.74%	0.437%
3	3.905	153	156	165	rVB2	19198	27929	0.55%	0.050%
4	4.834	312	314	321	rVB6	6260	9558	0.19%	0.017%
5	6.852	653	657	658	rBV3	18139	19146	0.37%	0.035%
6	6.893	659	664	675	rVB	215892	383181	7.50%	0.691%
7	7.046	684	690	700	rBV	861635	1373742	26.89%	2.477%
8	7.246	717	724	735	rBV	892654	1476053	28.89%	2.662%
9	7.710	796	803	813	rBV	951750	1544785	30.24%	2.786%
10	8.428	917	925	942	rBV	722972	1245165	24.37%	2.245%
11	8.869	992	1000	1009	rBV	988384	1649770	32.29%	2.975%
12	9.293	1063	1072	1076	rBV2	24165	40789	0.80%	0.074%
13	9.587	1114	1122	1134	rBV	801413	1351520	26.46%	2.437%
14	10.128	1204	1214	1227	rBV	1105724	2030836	39.75%	3.662%
15	10.498	1269	1277	1287	rBV	1399370	2351709	46.03%	4.241%
16	10.640	1294	1301	1324	rBV	804090	1722122	33.71%	3.105%
17	11.787	1487	1496	1501	rBV2	27766	47189	0.92%	0.085%
18	12.122	1547	1553	1561	rBV2	18273	35576	0.70%	0.064%
19	13.328	1755	1758	1763	rVB7	4657	5597	0.11%	0.010%
20	13.769	1826	1833	1849	rBV	2204876	3226920	63.17%	5.819%
21	14.045	1873	1880	1896	rBV	2596587	3837772	75.12%	6.921%
22	14.351	1926	1932	1940	rBV	2034856	3017046	59.06%	5.441%
23	14.416	1940	1943	1952	rVB	25606	51781	1.01%	0.093%
24	14.598	1968	1974	1990	rBV3	54966	185047	3.62%	0.334%
25	14.734	1995	1997	2001	rVB4	6119	6068	0.12%	0.011%
26	15.351	2092	2102	2117	rBV	3169056	4777139	93.51%	8.615%
27	15.475	2117	2123	2136	rVV	911592	1380570	27.02%	2.490%
28	15.592	2139	2143	2151	rVB3	18656	36821	0.72%	0.066%
29	15.839	2181	2185	2187	rBV5	5530	6669	0.13%	0.012%
30	16.092	2224	2228	2230	rVV5	3611	5218	0.10%	0.009%
31	16.133	2232	2235	2238	rVB4	4441	5398	0.11%	0.010%
32	16.592	2309	2313	2318	rVB5	10464	13808	0.27%	0.025%
33	16.892	2358	2364	2368	rBV4	6077	10479	0.21%	0.019%
34	17.098	2393	2399	2409	rBV	2169840	3101750	60.72%	5.593%
35	17.198	2409	2416	2434	rVV	3266743	4898344	95.88%	8.833%
36	17.657	2491	2494	2497	rVB4	6792	8689	0.17%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048339.D
Acq On : 31 Oct 2024 02:11
Operator : RC/JU
Sample : P4534-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L95

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	17.992	2548	2551	2562	rBV4	38325	69325	1.36%	0.125%
38	18.916	2706	2708	2711	rBV3	4632	5324	0.10%	0.010%
39	19.057	2728	2732	2736	rBV	34579	44422	0.87%	0.080%
40	19.127	2740	2744	2751	rBV2	35925	53445	1.05%	0.096%
41	19.274	2766	2769	2778	rBV8	34429	58473	1.14%	0.105%
42	19.492	2799	2806	2821	rBV	3582099	5108648	100.00%	9.212%
43	21.321	3111	3117	3129	rBV2	1702270	2757901	53.98%	4.973%
44	24.062	3574	3583	3598	rBV	1825200	4426174	86.64%	7.982%
45	24.262	3609	3617	3632	rVB	1090878	2726415	53.37%	4.917%




Sum of corrected areas: 55454044

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048339.D
Acq On : 31 Oct 2024 02:11
Operator : RC/JU
Sample : P4534-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L95

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

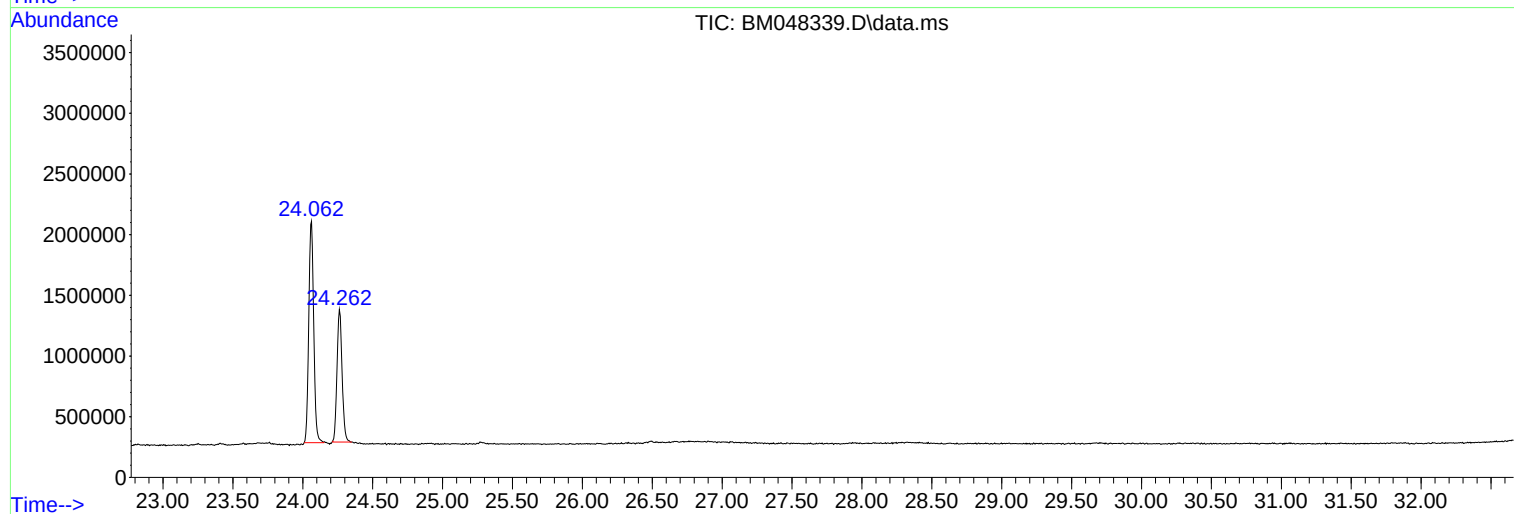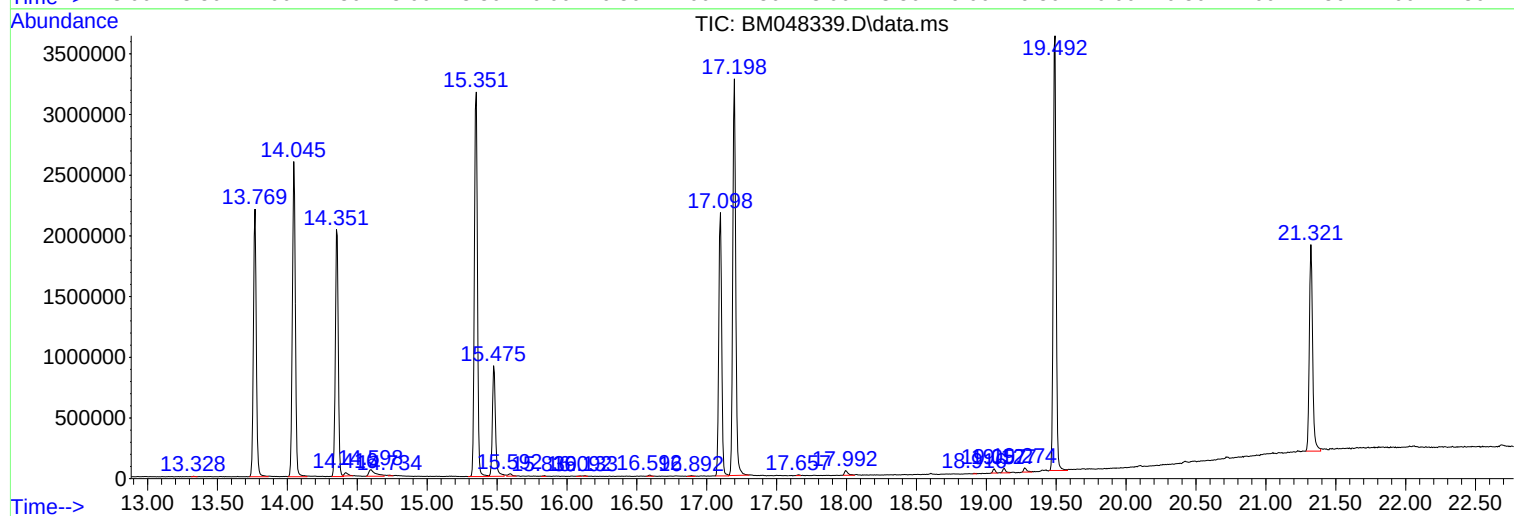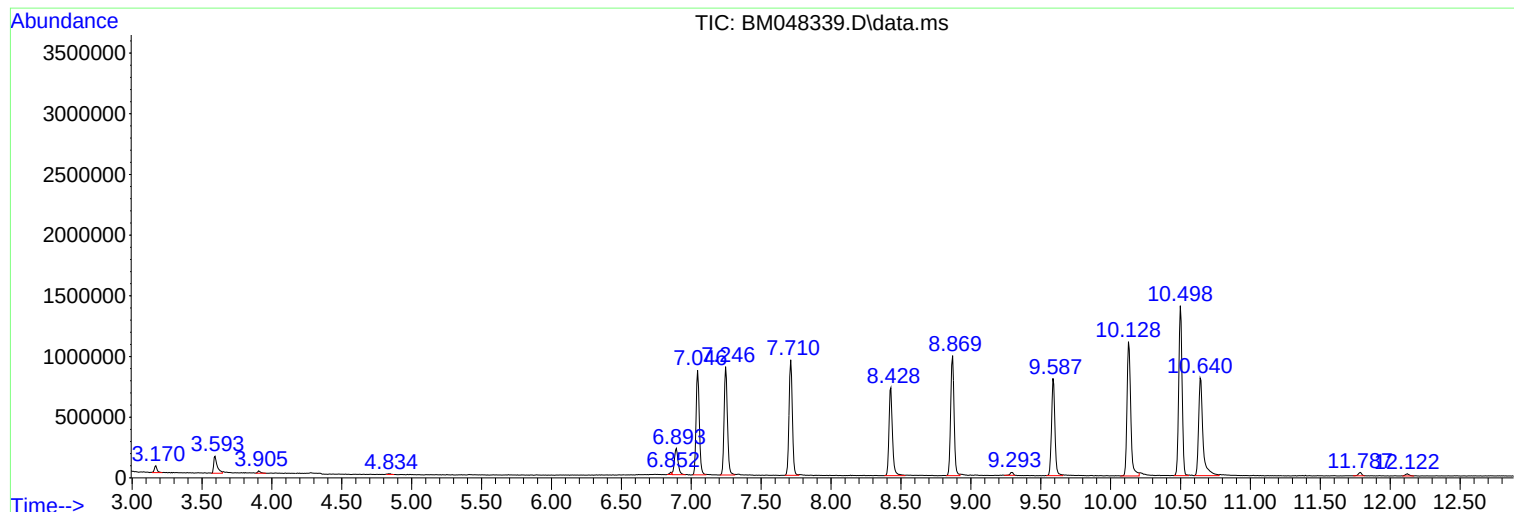

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048339.D
Acq On : 31 Oct 2024 02:11
Operator : RC/JU
Sample : P4534-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L95

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048339.D
Acq On : 31 Oct 2024 02:11
Operator : RC/JU
Sample : P4534-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L95

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
