

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048342.D
 Acq On : 31 Oct 2024 04:09
 Operator : RC/JU
 Sample : P4558-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L79

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048342.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	36	rBV	55664	72876	1.19%	0.112%
2	3.587	98	102	116	rBV	370925	585992	9.53%	0.897%
3	3.911	153	157	161	rVB4	13955	18489	0.30%	0.028%
4	4.816	308	311	316	rBV5	6710	12758	0.21%	0.020%
5	5.005	337	343	350	rVB	33186	53026	0.86%	0.081%
6	6.893	658	664	675	rVB	264215	468957	7.63%	0.718%
7	7.046	683	690	702	rBV	997572	1571613	25.57%	2.407%
8	7.246	717	724	735	rBV	1066767	1712119	27.86%	2.622%
9	7.340	737	740	748	rVB10	8143	13475	0.22%	0.021%
10	7.710	796	803	811	rBV	983894	1596028	25.97%	2.444%
11	7.781	814	815	820	rVB5	7024	8275	0.13%	0.013%
12	8.422	917	924	940	rBV	848321	1475155	24.00%	2.259%
13	8.869	992	1000	1013	rBV	1123257	1885683	30.68%	2.887%
14	9.293	1065	1072	1077	rVB	28808	50948	0.83%	0.078%
15	9.440	1093	1097	1106	rVB10	8188	21331	0.35%	0.033%
16	9.587	1115	1122	1133	rBV	921684	1547782	25.18%	2.370%
17	10.128	1206	1214	1237	rBV	1352355	2544763	41.40%	3.897%
18	10.498	1267	1277	1288	rBV	1461399	2410928	39.23%	3.692%
19	10.645	1293	1302	1320	rBV	640401	1392553	22.66%	2.132%
20	11.081	1371	1376	1379	rBV7	5469	10030	0.16%	0.015%
21	11.334	1414	1419	1429	rBV10	12488	38164	0.62%	0.058%
22	11.628	1464	1469	1475	rVB10	5610	9657	0.16%	0.015%
23	11.781	1488	1495	1503	rBV2	22822	46805	0.76%	0.072%
24	11.869	1506	1510	1514	rVB7	3678	6246	0.10%	0.010%
25	11.951	1520	1524	1531	rVB9	4229	9964	0.16%	0.015%
26	12.051	1535	1541	1547	rVV4	21893	58235	0.95%	0.089%
27	12.104	1547	1550	1557	rVB3	20406	35841	0.58%	0.055%
28	12.557	1622	1627	1628	rBV5	4677	7055	0.11%	0.011%
29	12.733	1652	1657	1662	rVB	41246	60744	0.99%	0.093%
30	13.181	1729	1733	1736	rBV6	9106	13449	0.22%	0.021%
31	13.251	1743	1745	1749	rVB5	6415	7379	0.12%	0.011%
32	13.363	1762	1764	1771	rVB7	9416	14822	0.24%	0.023%
33	13.428	1771	1775	1780	rBV8	4901	9927	0.16%	0.015%
34	13.692	1816	1820	1824	rVB4	11998	17240	0.28%	0.026%
35	13.769	1826	1833	1845	rBV	2727254	3793687	61.72%	5.809%
36	14.045	1872	1880	1897	rBV2	3051917	4601397	74.86%	7.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048342.D
Acq On : 31 Oct 2024 04:09
Operator : RC/JU
Sample : P4558-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	14.351	1926	1932	1948	rVB	2127571	3117137	50.71%	4.773%
38	14.592	1967	1973	1985	rBV2	105742	270897	4.41%	0.415%
39	15.351	2095	2102	2107	rBV	3795505	5619939	91.43%	8.605%
40	15.398	2107	2110	2117	rVV	181258	274012	4.46%	0.420%
41	15.474	2117	2123	2137	rVV	1281276	1808796	29.43%	2.770%
42	15.716	2159	2164	2171	rVB	140466	207703	3.38%	0.318%
43	16.574	2306	2310	2318	rVB4	57227	94494	1.54%	0.145%
44	16.698	2327	2331	2336	rVB	72761	95596	1.56%	0.146%
45	17.098	2393	2399	2405	rBV	2372160	3305669	53.78%	5.062%
46	17.198	2409	2416	2429	rBV	3897927	5776624	93.98%	8.845%
47	17.992	2547	2551	2561	rBV	194881	305501	4.97%	0.468%
48	18.274	2594	2599	2608	rBV	181531	263770	4.29%	0.404%
49	19.051	2728	2731	2736	rVB	50890	61907	1.01%	0.095%
50	19.127	2741	2744	2747	rVV	49030	55917	0.91%	0.086%
51	19.274	2765	2769	2778	rBV	108413	157656	2.57%	0.241%
52	19.486	2800	2805	2813	rBV	4590887	6146394	100.00%	9.412%
53	21.009	3061	3064	3073	rVB2	120959	189499	3.08%	0.290%
54	21.321	3111	3117	3130	rBV2	1916373	2963722	48.22%	4.538%
55	24.062	3574	3583	3603	rVB	2177600	5323749	86.62%	8.152%
56	24.262	3609	3617	3637	rVB	1182045	3084023	50.18%	4.722%




Sum of corrected areas: 65306398

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048342.D
Acq On : 31 Oct 2024 04:09
Operator : RC/JU
Sample : P4558-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L79

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

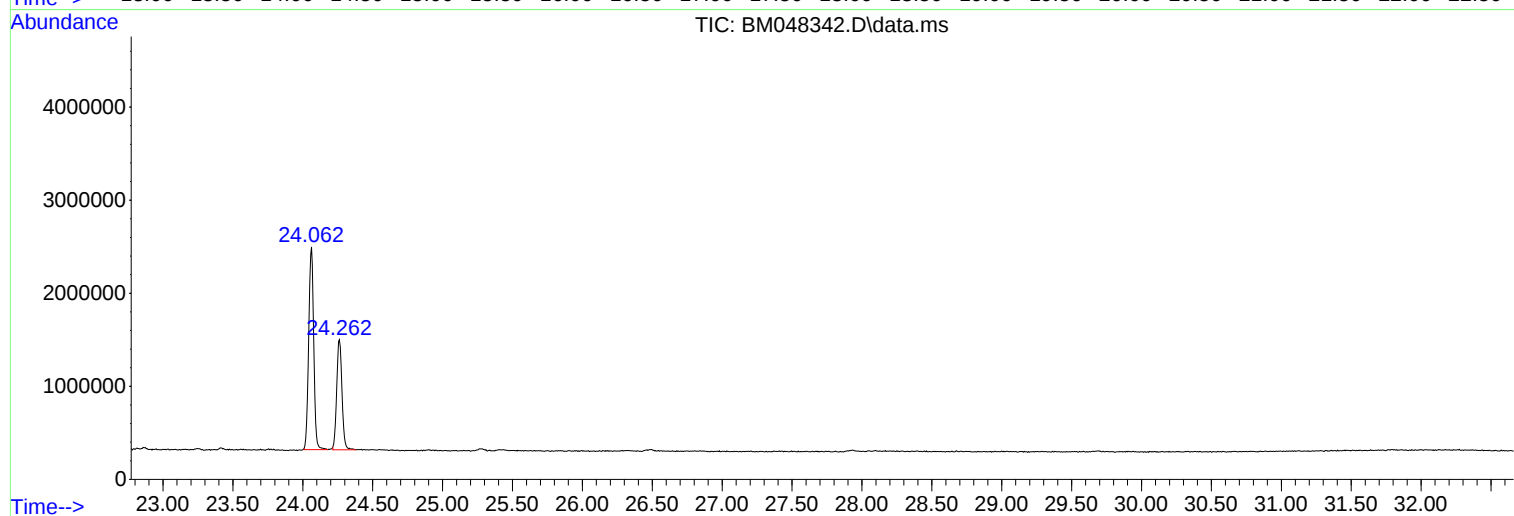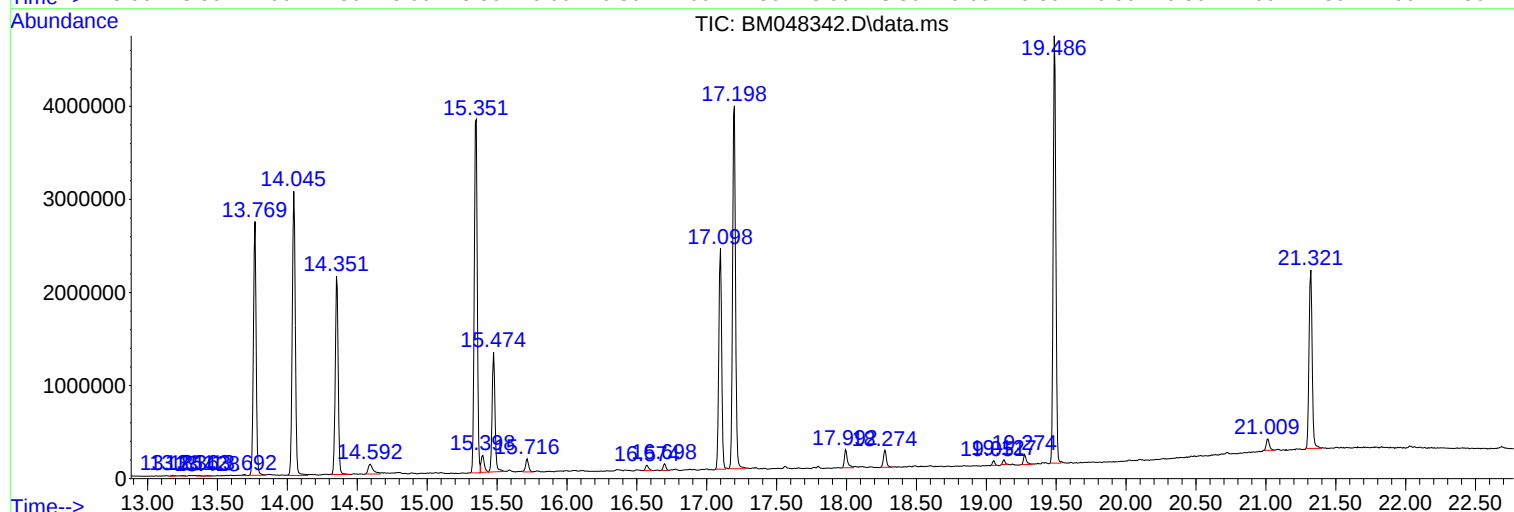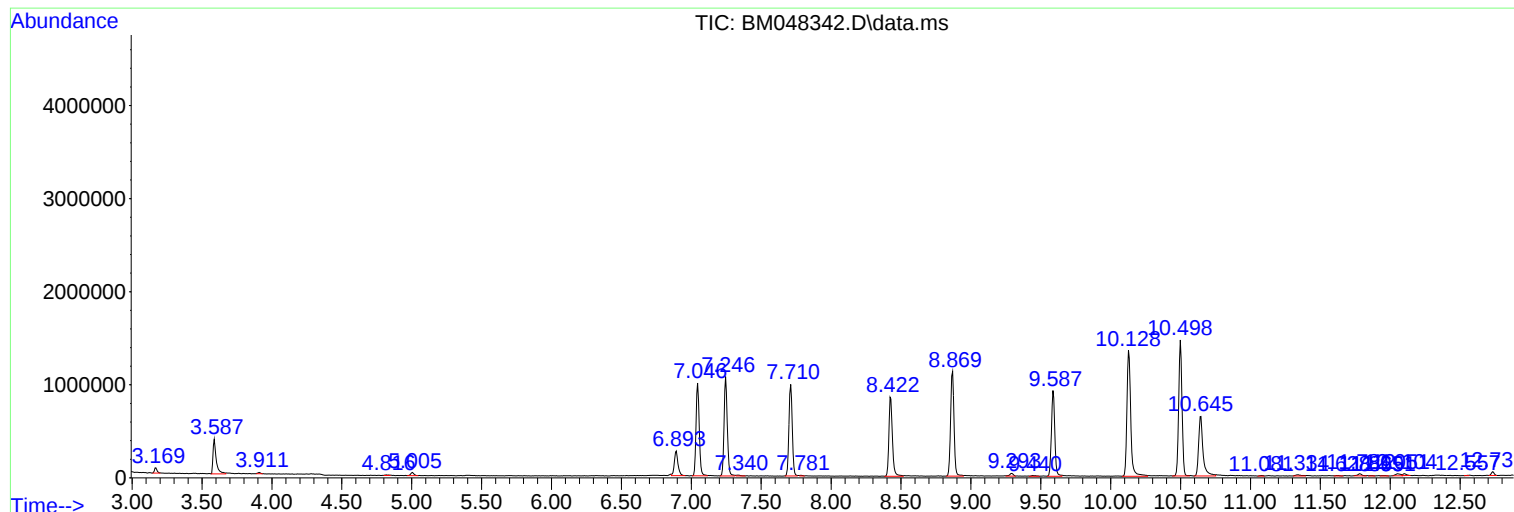

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048342.D
Acq On : 31 Oct 2024 04:09
Operator : RC/JU
Sample : P4558-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L79

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048342.D
Acq On : 31 Oct 2024 04:09
Operator : RC/JU
Sample : P4558-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L79

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc