

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102918\
 Data File : BM017417.D
 Acq On : 29 Oct 2018 21:16
 Operator : MJ/SJ
 Sample : J5706-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 30 02:53:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 29 15:08:36 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	234738	20.00	ng	0.00
21) Naphthalene-d8	10.42	136	1029259	20.00	ng	0.00
39) Acenaphthene-d10	14.29	164	635127	20.00	ng	0.00
64) Phenanthrene-d10	17.04	188	1651957	20.00	ng	0.00
76) Chrysene-d12	21.24	240	1773545	20.00	ng	0.00
87) Perylene-d12	23.44	264	1616497	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	571059	41.15	ng	0.00
7) Phenol-d6	6.83	99	476520	25.21	ng	0.00
23) Nitrobenzene-d5	8.80	82	1781434	101.23	ng	0.00
42) 2,4,6-Tribromophenol	15.79	330	957597	111.49	ng	0.00
45) 2-Fluorobiphenyl	12.90	172	4633085	97.06	ng	0.00
79) Terphenyl-d14	19.69	244	7353149	93.45	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.76	163	215344	4.395	ng	99
80) Butylbenzylphthalate	20.39	149	1355	7.206	ng	# 77
84) Bis(2-ethylhexyl)phthalate	21.16	149	3573	5.363	ng	# 90
85) Di-n-octyl phthalate	22.03	149	2210	5.591	ng	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102918\
Data File : BM017417.D
Acq On : 29 Oct 2018 21:16
Operator : MJ/SJ
Sample : J5706-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 30 02:53:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 29 15:08:36 2018
Response via : Initial Calibration

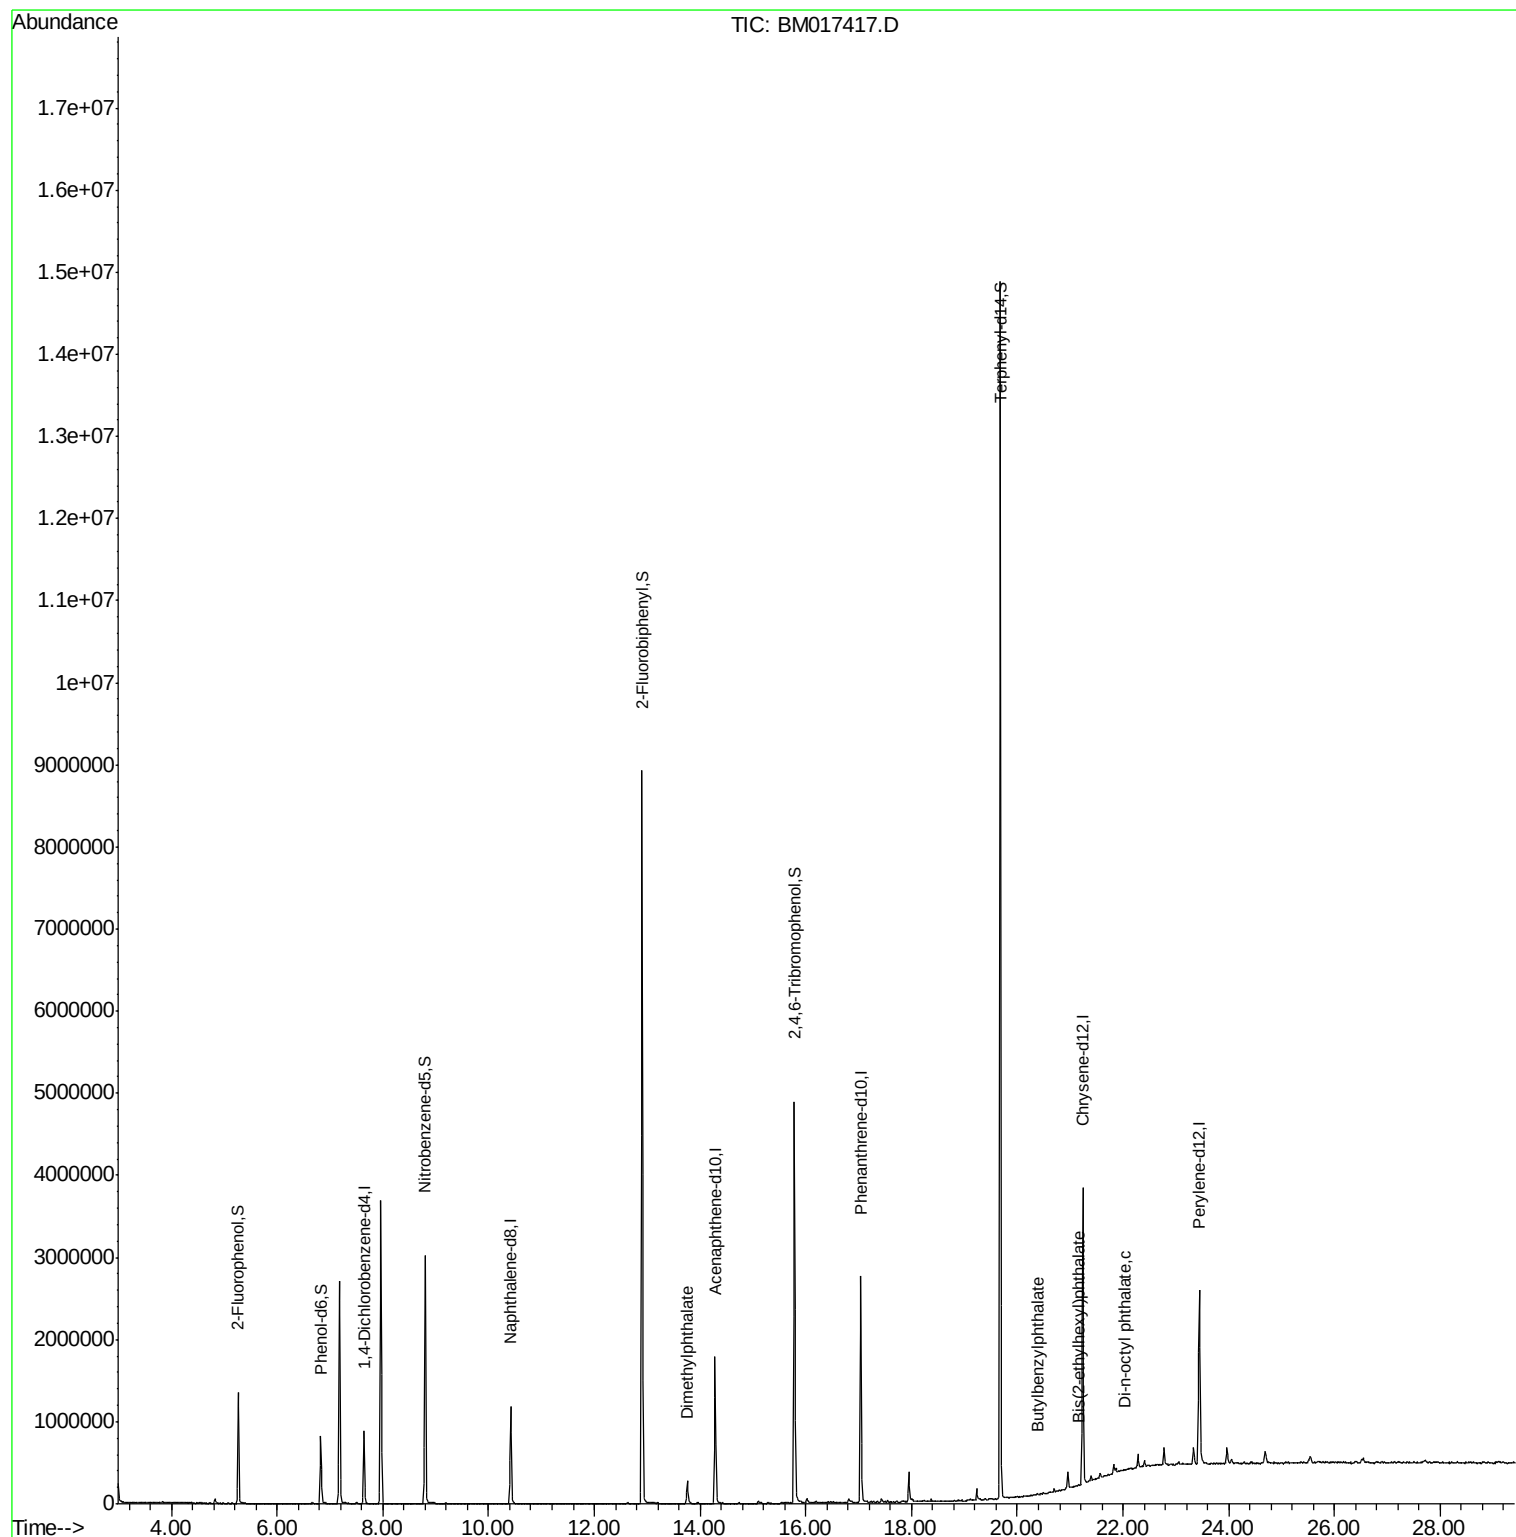




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.65 min Scan# 792
Delta R.T. -0.00 min
Lab File: BM017417.D
Acq: 29 Oct 2018 21:16

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.8	124.3	186.5
115	62.4	48.1	72.1






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

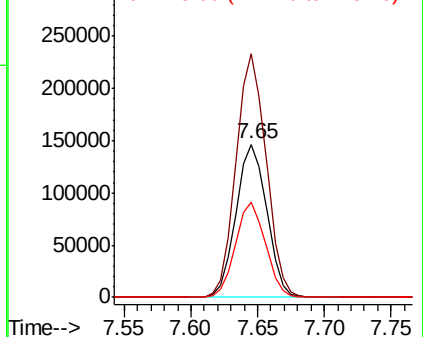

#5

2-Fluorophenol
Concen: 41.146 ng
RT: 5.26 min Scan# 387
Delta R.T. -0.00 min
Lab File: BM017417.D
Acq: 29 Oct 2018 21:16

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.0	41.7	62.5
63	29.7	23.0	34.4






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

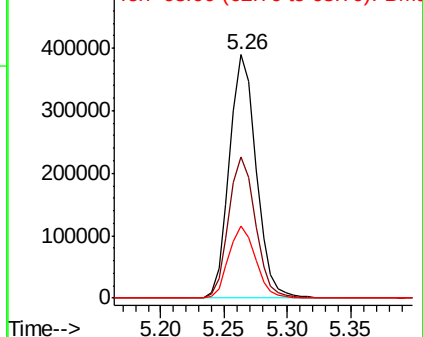

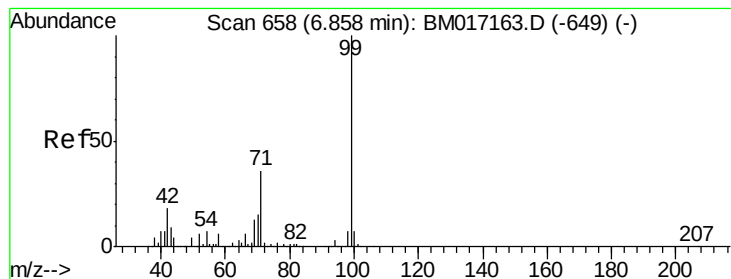

#7

Phenol-d6

Concen: 25.210 ng

RT: 6.83 min Scan# 653

Delta R.T. -0.01 min

Lab File: BM017417.D

Acq: 29 Oct 2018 21:16

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 99 Resp: 476520

Ion Ratio Lower Upper

99 100

42 17.0 13.3 19.9




71 35.9 28.0 42.0



Abundance Ion 99.00 (98.70 to 99.70): BM017163.D (-649) (-)

Ion 42.00 (41.70 to 42.70): BM017163.D (-649) (-)

Ion 71.00 (70.70 to 71.70): BM017163.D (-649) (-)

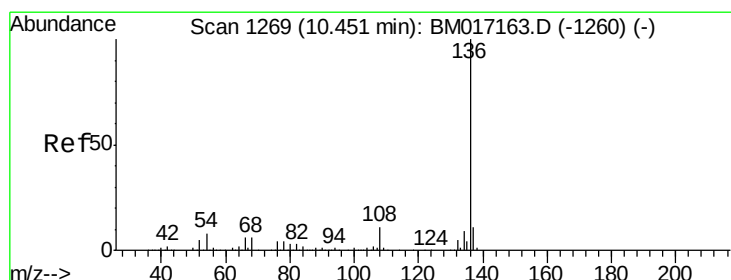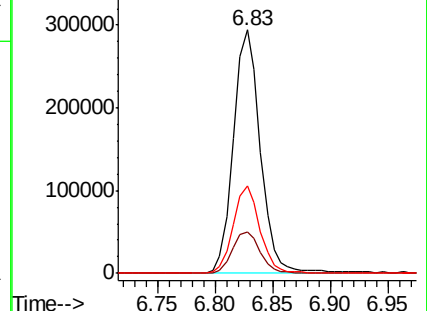

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.42 min Scan# 1264

Delta R.T. -0.00 min

Lab File: BM017417.D

Acq: 29 Oct 2018 21:16

Tgt Ion: 136 Resp: 1029259


Ion Ratio Lower Upper

136 100

137 10.4 9.2 13.8

54 7.6 6.7 10.1

68 5.8 4.7 7.1






Abundance Ion 136.00 (135.70 to 136.70): BM017163.D (-1260) (-)

Ion 137.00 (136.70 to 137.70): BM017163.D (-1260) (-)

Ion 54.00 (53.70 to 54.70): BM017163.D (-1260) (-)

Ion 68.00 (67.70 to 68.70): BM017163.D (-1260) (-)

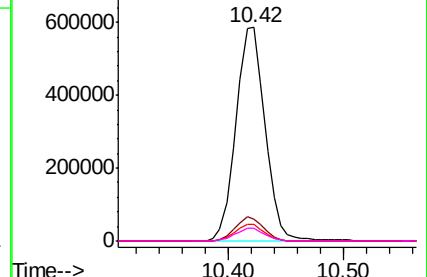







#23
 Nitrobenzene-d5
 Concen: 101.227 ng
 RT: 8.80 min Scan# 988
 Delta R.T. -0.01 min
 Lab File: BM017417.D
 Acq: 29 Oct 2018 21:16

Instrument :
 BNA_M
 ClientSampled :

Tot Ion: 82 Resp: 1781434
 Ion Ratio Lower Upper
 82 100
 128 43.7 37.0 55.6
 54 48.8 40.7 61.1

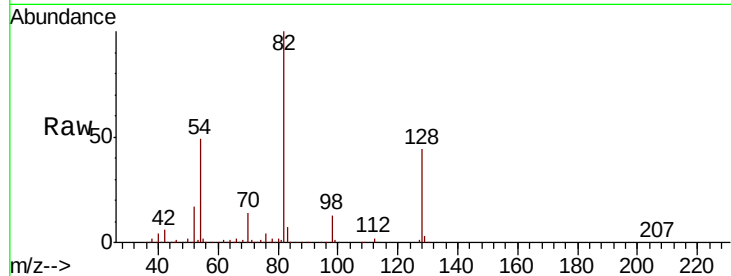


Abundance Ion 82.00 (81.70 to 82.70): BM0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BM0


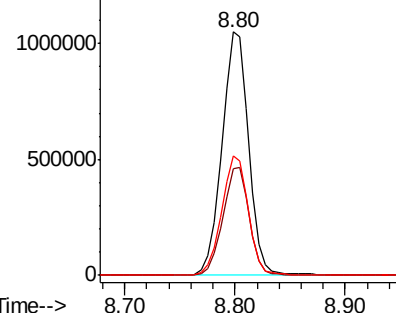



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.29 min Scan# 1921
 Delta R.T. -0.01 min
 Lab File: BM017417.D
 Acq: 29 Oct 2018 21:16

Tgt Ion:164 Resp: 635127
 Ion Ratio Lower Upper
 164 100
 162 100.5 82.1 123.1
 160 45.0 40.2 60.2



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

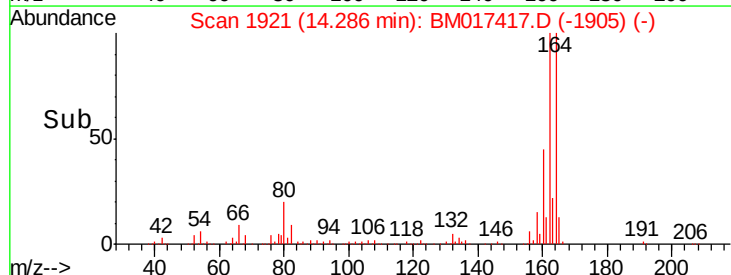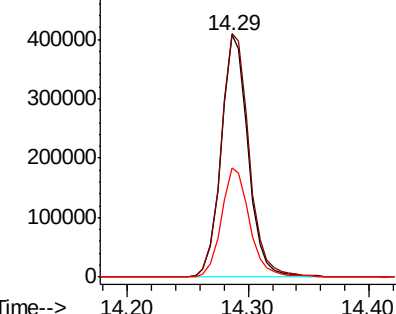




#42
 2,4,6-Tribromophenol
 Concen: 111.489 ng
 RT: 15.79 min Scan# 2176
 Delta R.T. -0.01 min
 Lab File: BM017417.D
 Acq: 29 Oct 2018 21:16

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	77.3	115.9
141	32.9	27.4	41.0



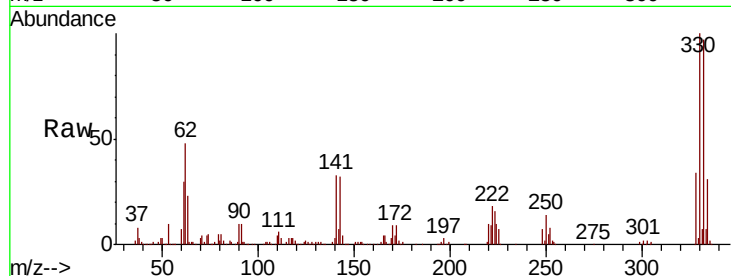


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

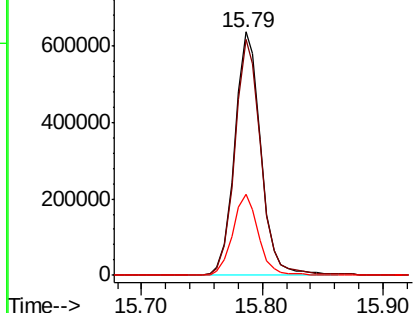

#45
 2-Fluorobiphenyl
 Concen: 97.060 ng
 RT: 12.90 min Scan# 1686
 Delta R.T. -0.00 min
 Lab File: BM017417.D
 Acq: 29 Oct 2018 21:16

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.1	28.3	42.5
170	22.6	18.3	27.5






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

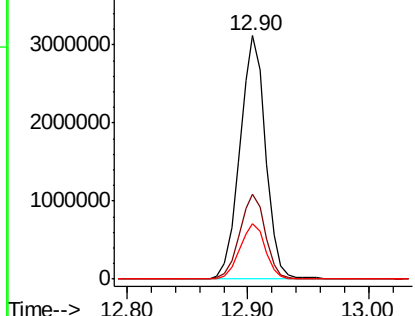


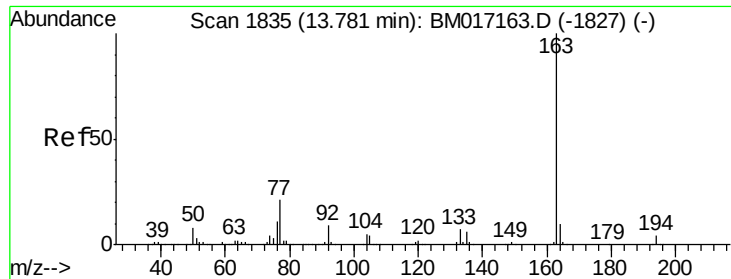




#50
Dimethylphthalate
Concen: 4.395 ng
RT: 13.76 min Scan# 1831
Delta R.T. -0.01 min
Lab File: BM017417.D
Acq: 29 Oct 2018 21:16

Instrument :
BNA_M
ClientSampleId :

Tot Ion:163 Resp: 215344
Ion Ratio Lower Upper
163 100
194 4.0 3.3 4.9
164 10.2 7.8 11.8




Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

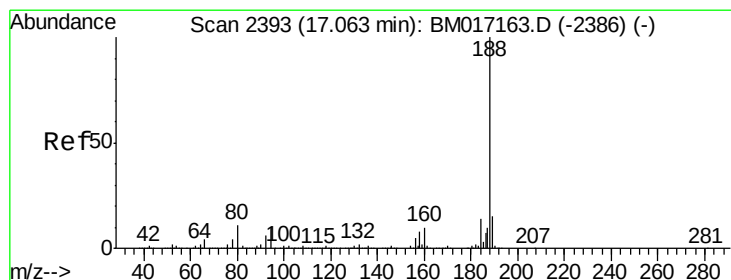
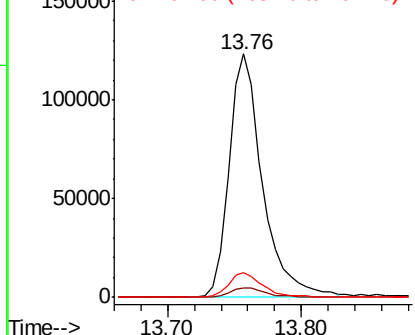



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.04 min Scan# 2389
Delta R.T. -0.01 min
Lab File: BM017417.D
Acq: 29 Oct 2018 21:16

Tgt Ion:188 Resp: 1651957
Ion Ratio Lower Upper
188 100
94 8.9 7.0 10.4
80 10.2 7.7 11.5

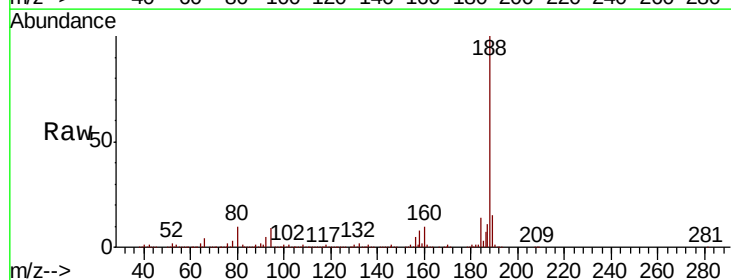

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0




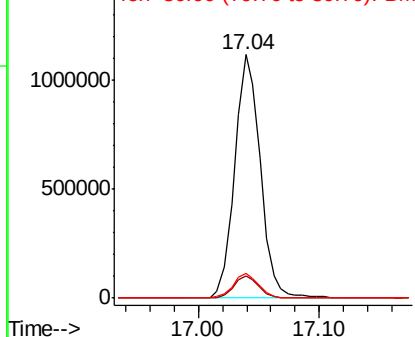


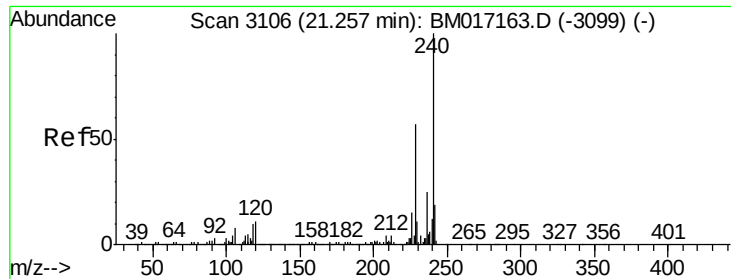

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.24 min Scan# 3103
 Delta R.T. -0.01 min
 Lab File: BM017417.D
 Acq: 29 Oct 2018 21:16




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:240 Resp: 1773545
 Ion Ratio Lower Upper
 240 100
 120 10.0 8.1 12.1
 236 25.0 19.9 29.9

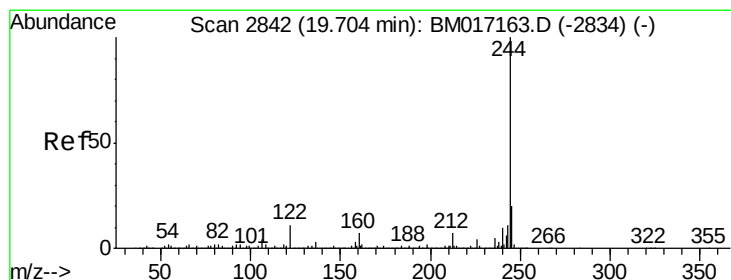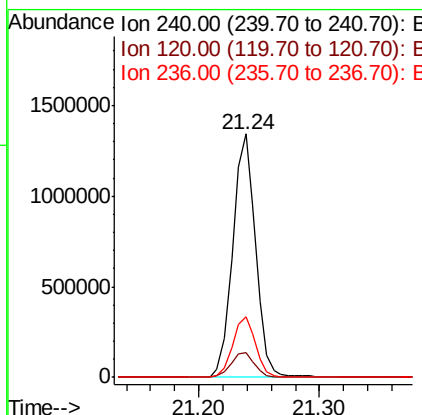

#79
 Terphenyl-d14
 Concen: 93.451 ng
 RT: 19.69 min Scan# 2839
 Delta R.T. -0.00 min
 Lab File: BM017417.D
 Acq: 29 Oct 2018 21:16

Tgt Ion:244 Resp: 7353149
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.5 8.3
 122 10.3 8.4 12.6



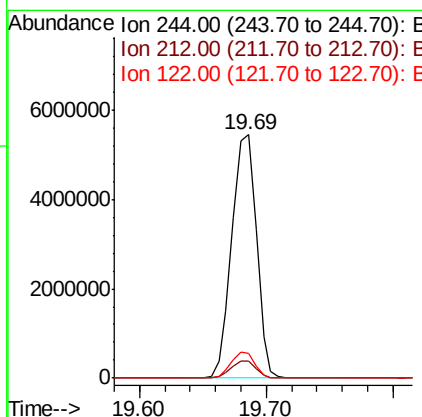





#80
 Butylbenzylphthalate
 Concen: 7.206 ng
 RT: 20.39 min Scan# 2959
 Delta R.T. 0.01 min
 Lab File: BM017417.D
 Acq: 29 Oct 2018 21:16




Instrument :
 BNA_M
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
149	100		
91	75.5	51.3	76.9
206	0.0	18.0	27.0

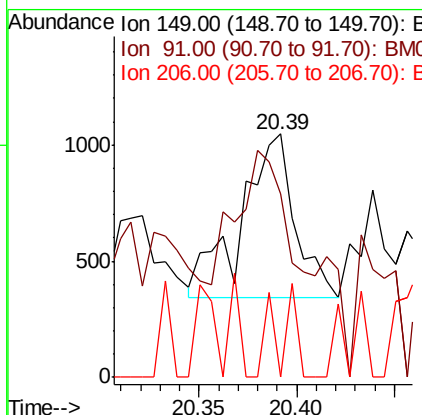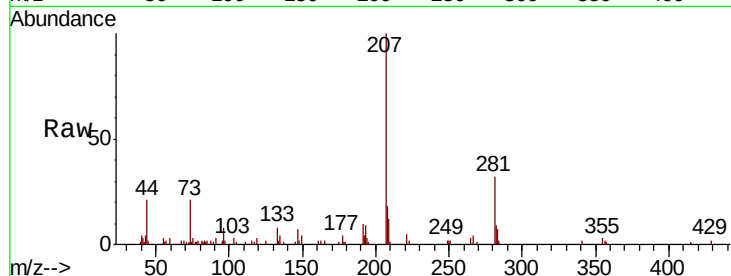

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 5.363 ng
 RT: 21.16 min Scan# 3090
 Delta R.T. -0.00 min
 Lab File: BM017417.D
 Acq: 29 Oct 2018 21:16

Tgt Ion	Ratio	Lower	Upper
149	100		
167	23.0	22.2	33.4
279	0.0	3.6	5.4



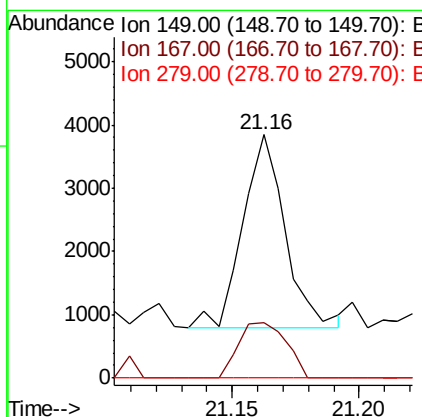



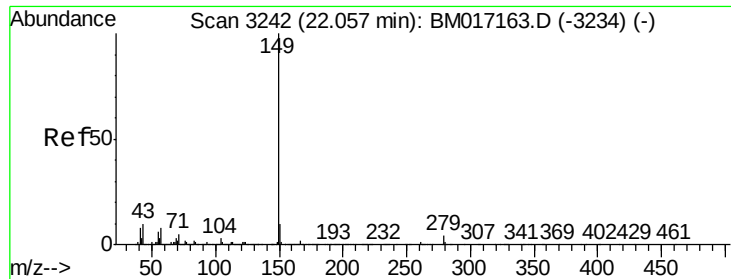

#85
Di-n-octyl phthalate
Concen: 5.591 ng
RT: 22.03 min Scan# 3238
Delta R.T. -0.01 min
Lab File: BM017417.D
Acq: 29 Oct 2018 21:16

Instrument :
BNA_M
ClientSampled :

Tot Ion:149 Resp: 2210
Ion Ratio Lower Upper
149 100
167 17.5 1.4 2.0#
43 10.6 7.2 10.8

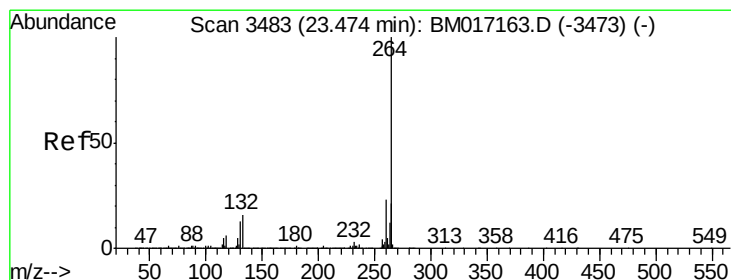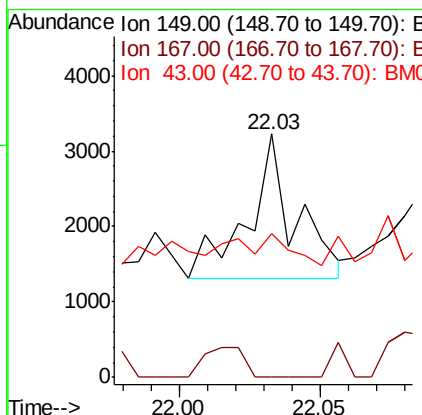

#87
Perylene-d12
Concen: 20.000 ng
RT: 23.44 min Scan# 3478
Delta R.T. -0.01 min
Lab File: BM017417.D
Acq: 29 Oct 2018 21:16

Tgt Ion:264 Resp: 1616497
Ion Ratio Lower Upper
264 100
260 23.3 18.6 27.8
265 22.0 17.8 26.8

