


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM102918\
 Data File : BM017401.D
 Acq On : 29 Oct 2018 10:47
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 29 15:08:36 2018

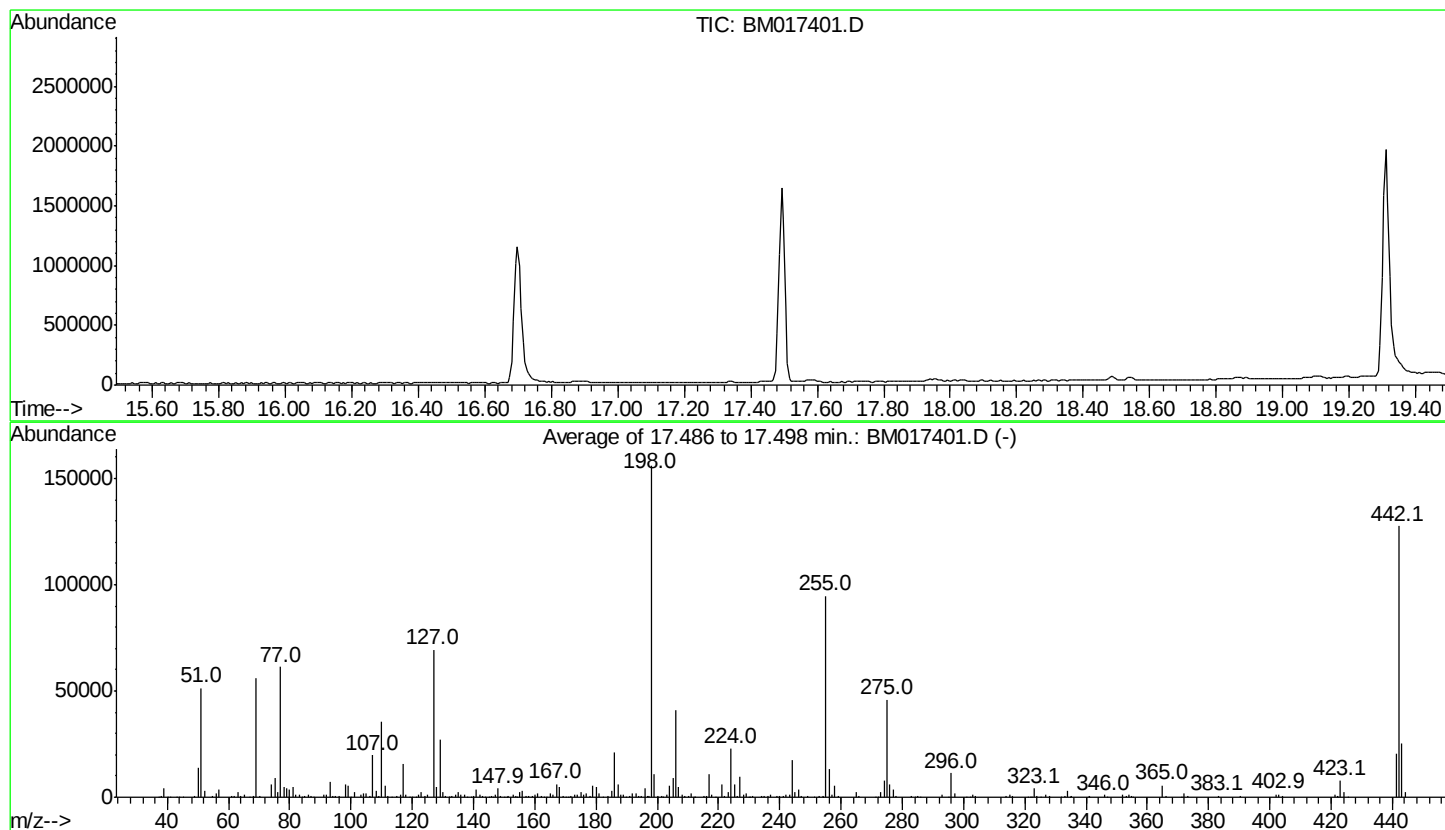

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	51445	PASS
68	69	0.00	2	1.4	762	PASS
69	198	0.00	100	36.1	56290	PASS
70	69	0.00	2	0.9	495	PASS
127	198	10	80	44.4	69320	PASS
197	198	0.00	2	0.5	715	PASS
198	198	100	100	100.0	156086	PASS
199	198	5	9	7.0	10851	PASS
275	198	10	60	29.4	45842	PASS
365	198	1	100	3.5	5492	PASS
441	198	0.01	100	13.1	20405	PASS
442	198	50	100	81.8	127698	PASS
443	442	15	24	19.8	25282	PASS