


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM102918\
 Data File : BM017410.D
 Acq On : 29 Oct 2018 17:04
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 29 15:08:36 2018

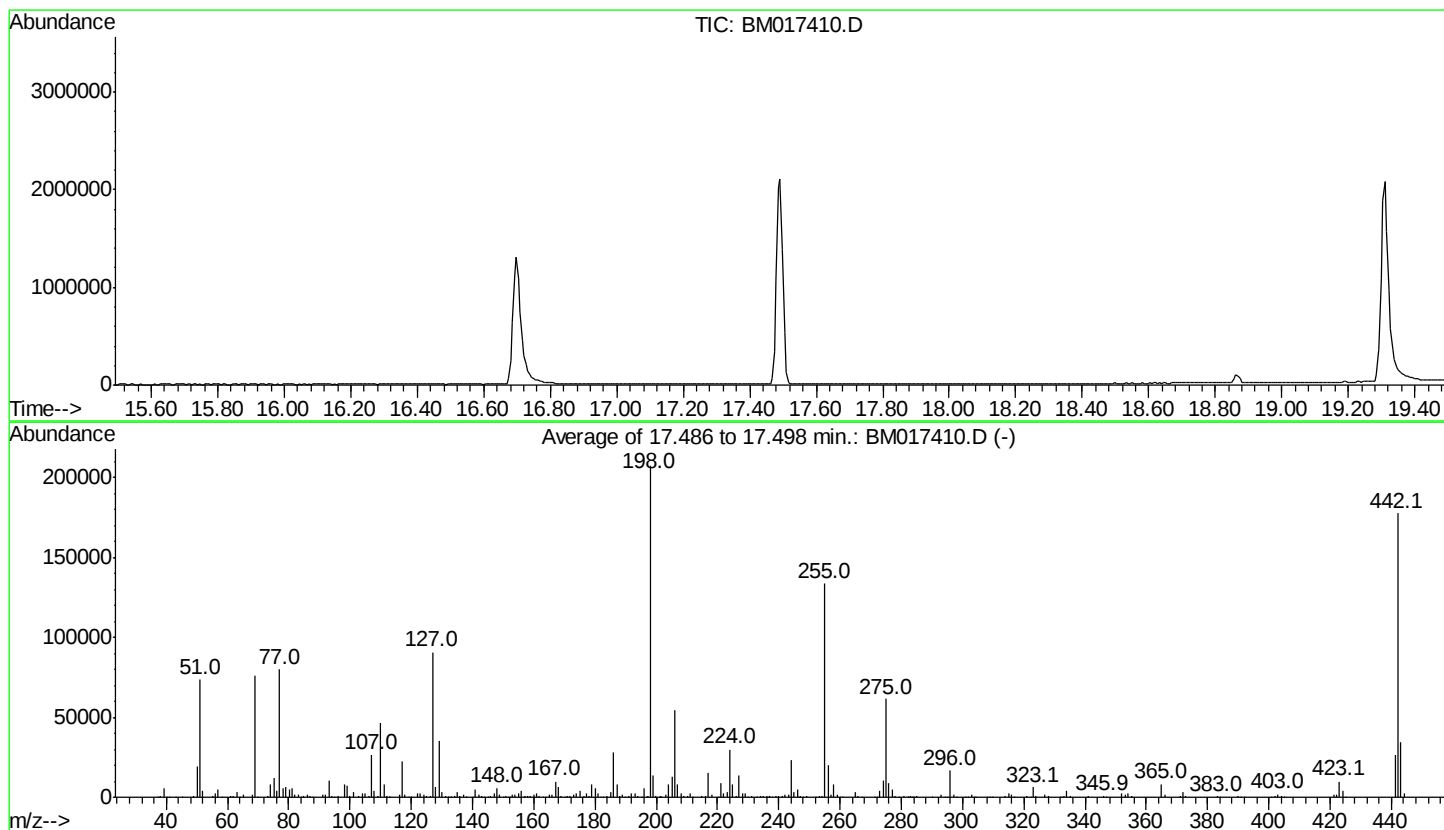

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	73392	PASS
68	69	0.00	2	1.8	1359	PASS
69	198	0.00	100	36.8	76336	PASS
70	69	0.00	2	0.5	380	PASS
127	198	10	80	43.6	90453	PASS
197	198	0.00	2	0.4	914	PASS
198	198	100	100	100.0	207338	PASS
199	198	5	9	6.5	13430	PASS
275	198	10	60	29.7	61536	PASS
365	198	1	100	3.9	8066	PASS
441	198	0.01	100	12.8	26509	PASS
442	198	50	100	85.5	177365	PASS
443	442	15	24	19.2	34106	PASS