

Data File : BM023504.D
Acq On : 31 Oct 2019 05:02
Operator : JU
Sample : K5487-13
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJK8

Quant Time: Oct 31 06:49:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 31 06:46:10 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	604508	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	2375043	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	1467369	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.01	188	2981973	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	2954671	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	3365858	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	59789	4.70	ng/uL	0.00
5) Phenol-d5	6.80	99	250053	4.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	622753	20.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	685360	17.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	455102	11.04	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	417461	23.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	449775	22.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	823484	21.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	44389	0.99	ng/ul	0.00
44) Dimethylphthalate-d6	13.68	166	2882581	25.87	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	3158481	24.74	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	102858	5.33	ng/ul	0.01
58) Fluorene-d10	15.26	176	2448330	25.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	394271	21.24	ng/ul	0.00
71) Anthracene-d10	17.11	188	3955406	28.07	ng/ul	0.00
79) Pyrene-d10	19.41	212	4270993	26.28	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	4923393	28.71	ng/ul	0.00

Target Compounds


					Qvalue
2) 1,4-Dioxane	3.18	88	23923	1.766 ng/uL	96
4) Benzaldehyde	6.77	77	34113	1.167 ng/ul#	1
6) Phenol	6.82	94	88747	1.697 ng/ul	99
14) Acetophenone	8.42	105	83811	1.301 ng/ul#	42
28) Naphthalene	10.45	128	7673585	63.037 ng/ul	100
34) 2-Methylnaphthalene	12.06	142	703589	7.566 ng/ul	97
35) 1-Methylnaphthalene	12.29	142	1632615	18.194 ng/ul	99
45) Dimethylphthalate	13.73	163	351031	3.138 ng/ul	99
50) Acenaphthene	14.33	153	613286	6.589 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM023504.D
Acq On : 31 Oct 2019 05:02
Operator : JU
Sample : K5487-13
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJK8

Quant Time: Oct 31 06:49:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 31 06:46:10 2019
Response via : Initial Calibration

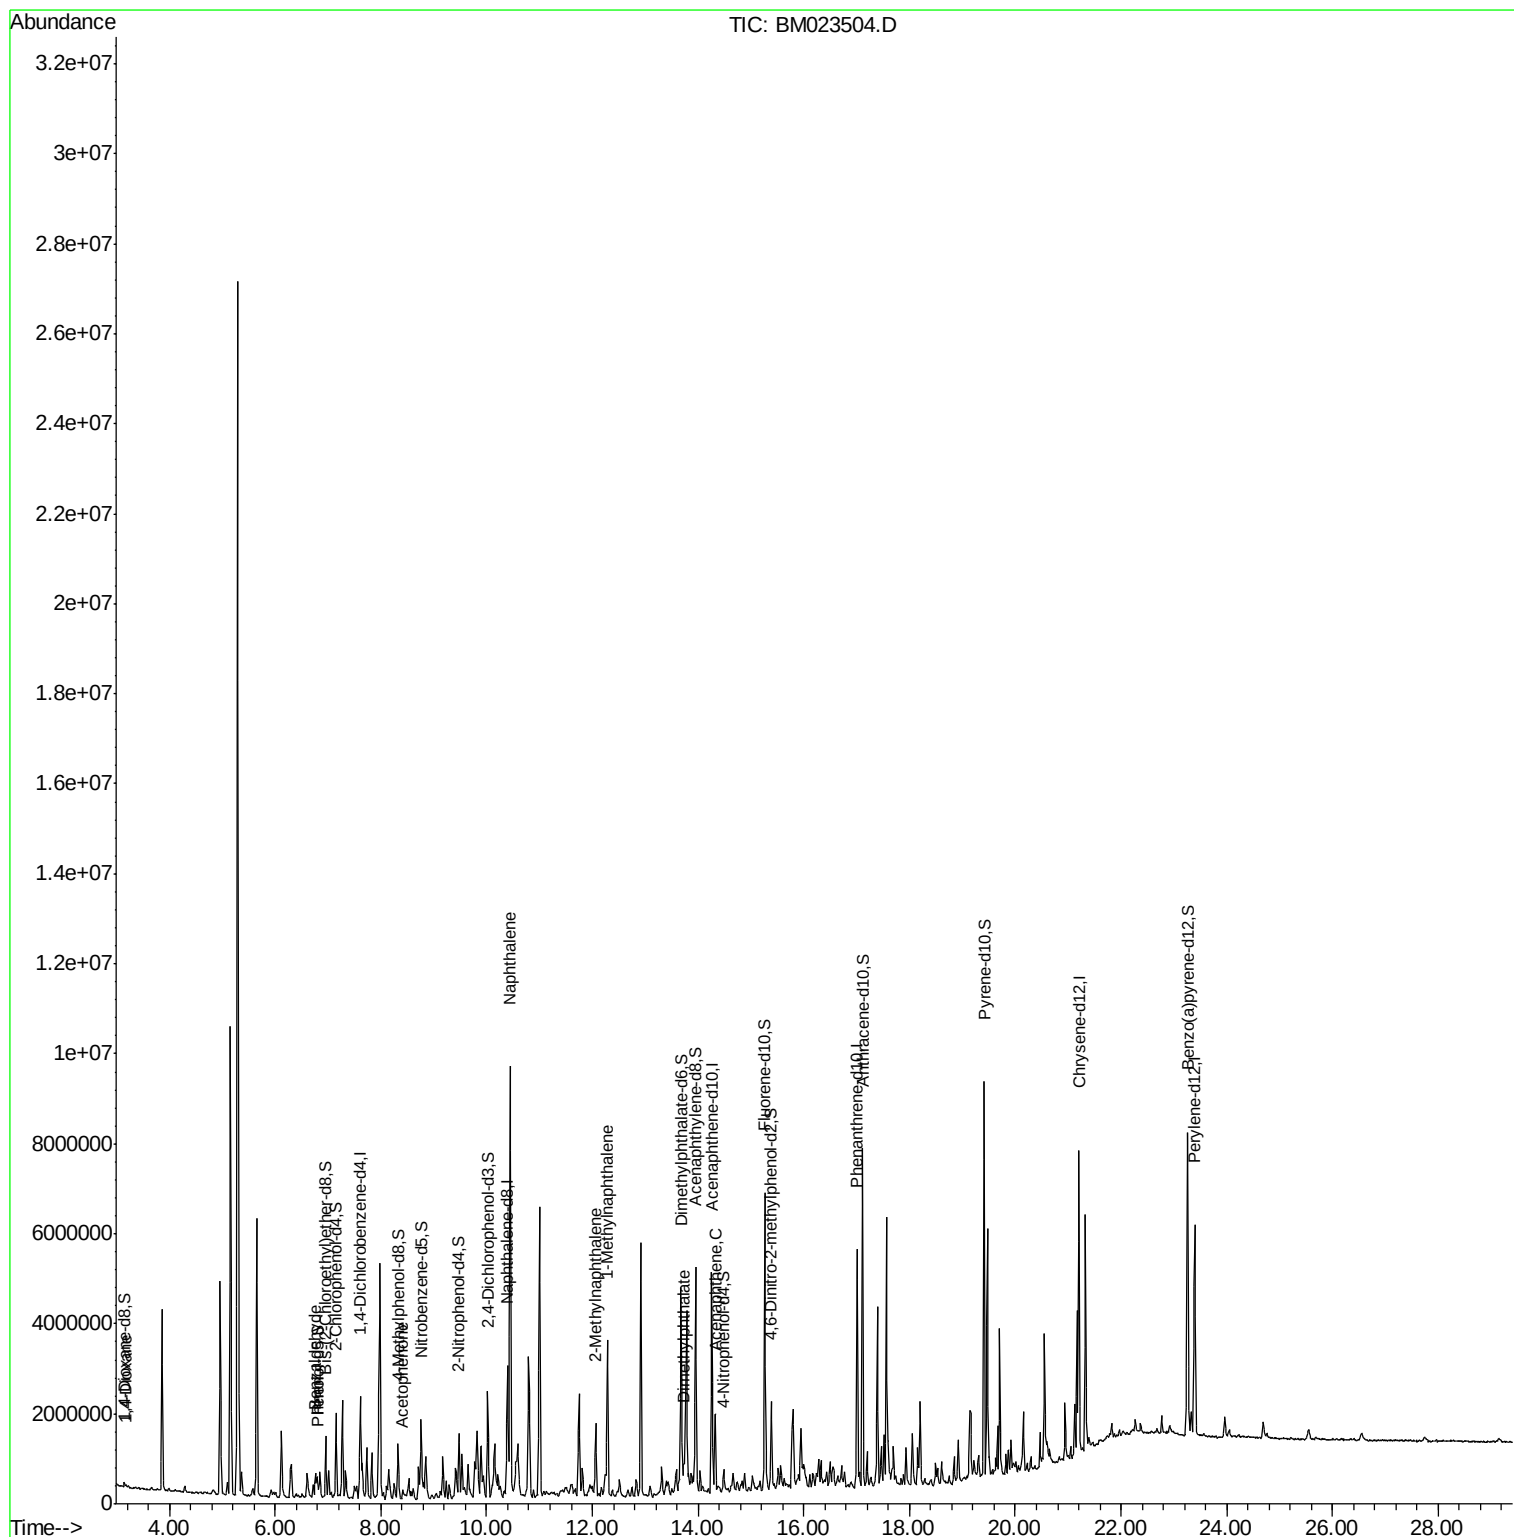

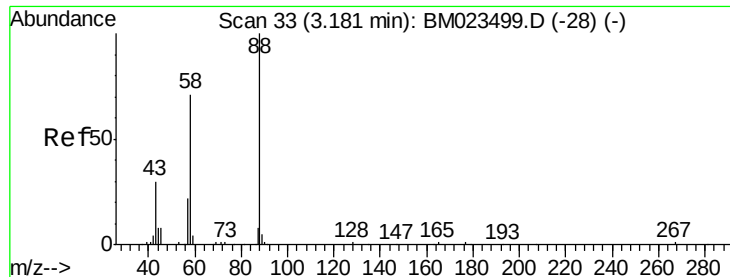

#2

1,4-Dioxane

Concen: 1.766 ng/uL

RT: 3.18 min Scan# 33

Delta R.T. -0.00 min

Lab File: BM023504.D

Acq: 31 Oct 2019 05:02

Instrument :

BNA_M

ClientSampleId :

BEJK8


Tgt Ion: 88 Resp: 23923

Ion Ratio Lower Upper

88 100

43 38.2 26.3 39.5




58 70.7 58.0 87.0

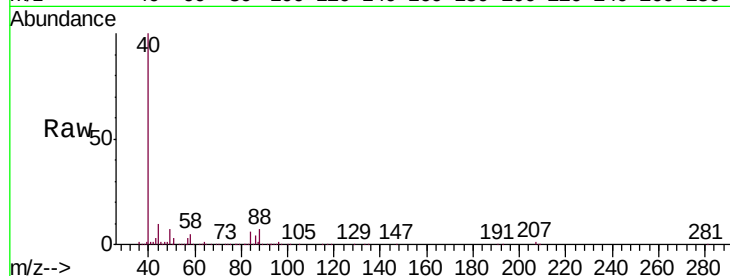

Abundance Ion 88.00 (87.70 to 88.70): BM023499.D (-28) (-)

Ion 43.00 (42.70 to 43.70): BM023499.D (-28) (-)

Ion 58.00 (57.70 to 58.70): BM023499.D (-28) (-)

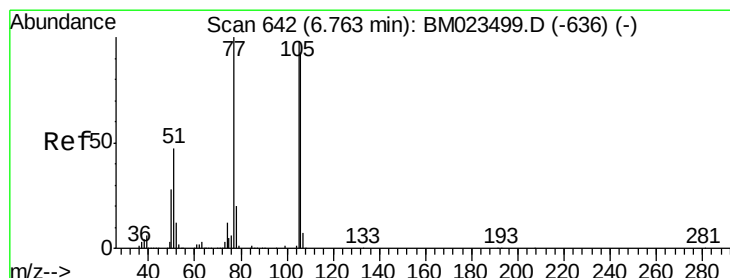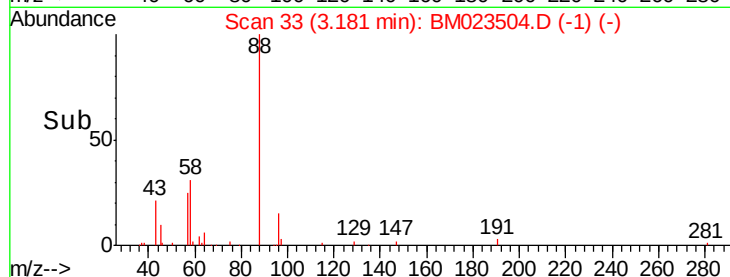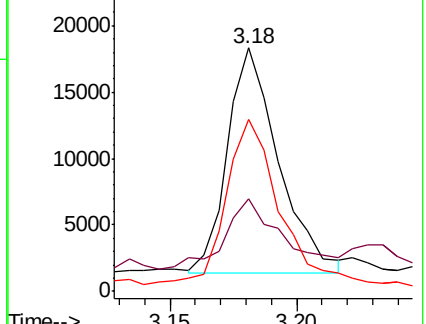

#4

Benzaldehyde

Concen: 1.167 ng/uL

RT: 6.77 min Scan# 643

Delta R.T. 0.01 min

Lab File: BM023504.D

Acq: 31 Oct 2019 05:02


Tgt Ion: 77 Resp: 34113

Ion Ratio Lower Upper

77 100

105 239.7 75.4 113.2#



106 36.4 71.3 106.9#

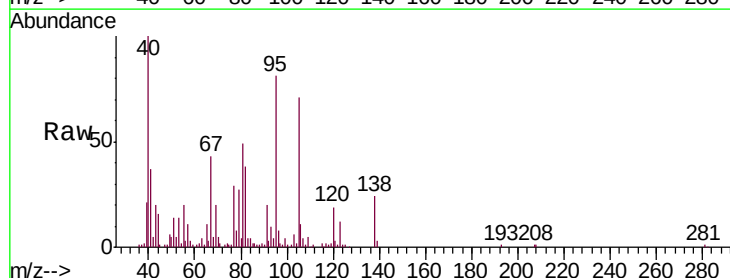


Abundance Ion 77.00 (76.70 to 77.70): BM023499.D (-636) (-)

Ion 105.00 (104.70 to 105.70): BM023499.D (-636) (-)

Ion 106.00 (105.70 to 106.70): BM023499.D (-636) (-)

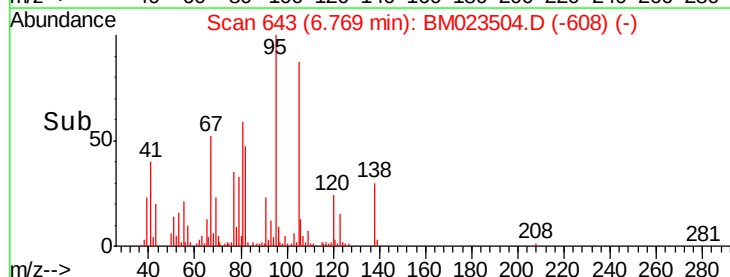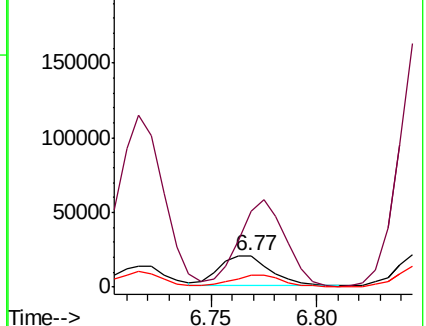

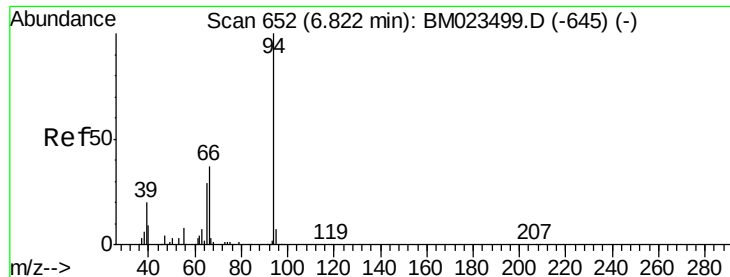

#6

Phenol

Concen: 1.697 ng/ul

RT: 6.82 min Scan# 652

Delta R.T. -0.00 min

Lab File: BM023504.D

Acq: 31 Oct 2019 05:02

Instrument :

BNA_M

ClientSampleId :

BEJK8


Tgt Ion: 94 Resp: 88747

Ion Ratio Lower Upper




94 100

65 27.7 22.9 34.3

66 38.7 31.4 47.2

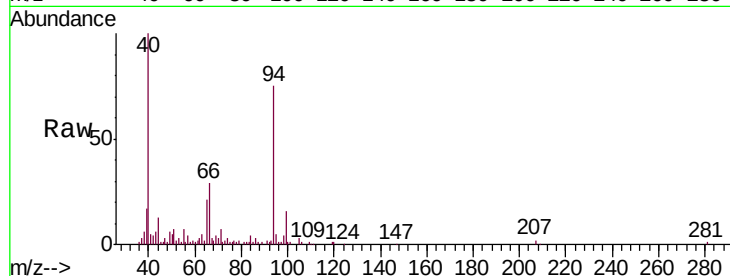

Abundance Ion 94.00 (93.70 to 94.70): BMC
Ion 65.00 (64.70 to 65.70): BMC
Ion 66.00 (65.70 to 66.70): BMC

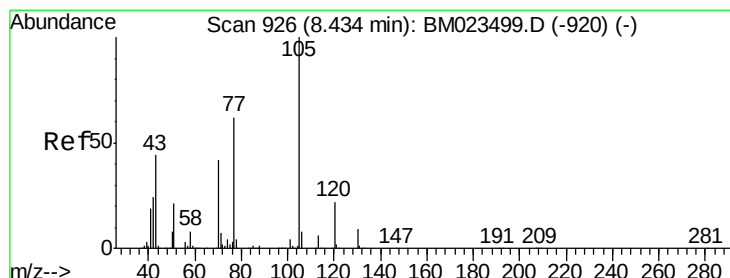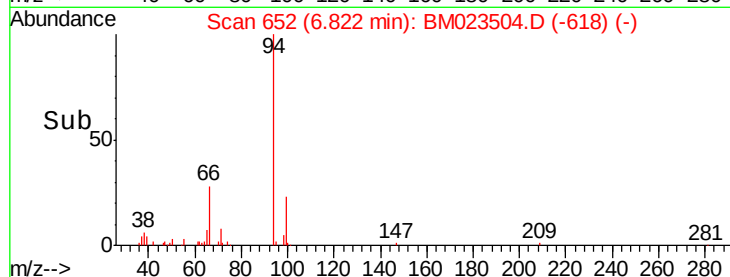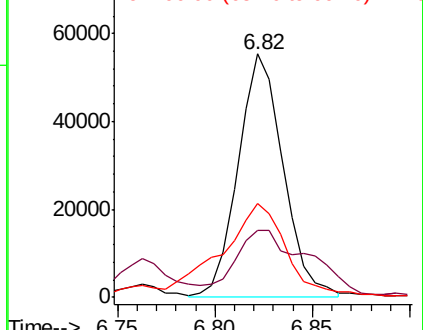

#14

Acetophenone

Concen: 1.301 ng/ul

RT: 8.42 min Scan# 924

Delta R.T. -0.01 min

Lab File: BM023504.D

Acq: 31 Oct 2019 05:02


Tgt Ion: 105 Resp: 83811

Ion Ratio Lower Upper



105 100


77 21.9 64.8 97.2#

51 11.0 21.3 31.9#

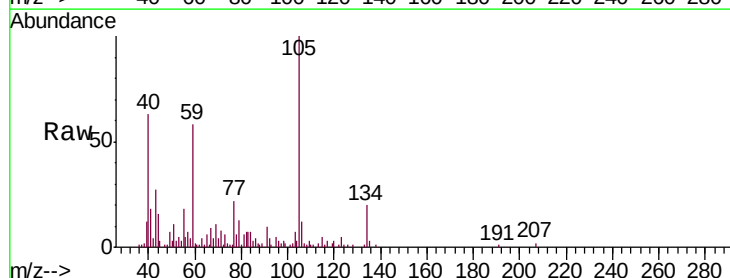

Abundance Ion 105.00 (104.70 to 105.70): BMC
Ion 77.00 (76.70 to 77.70): BMC
Ion 51.00 (50.70 to 51.70): BMC

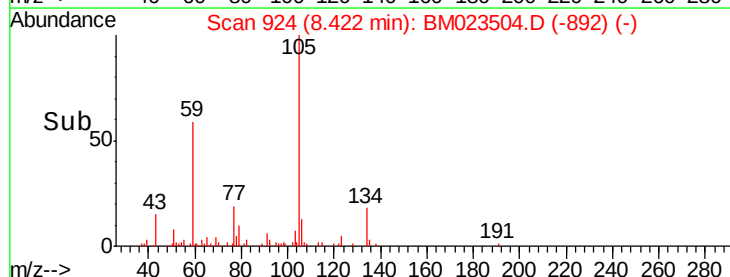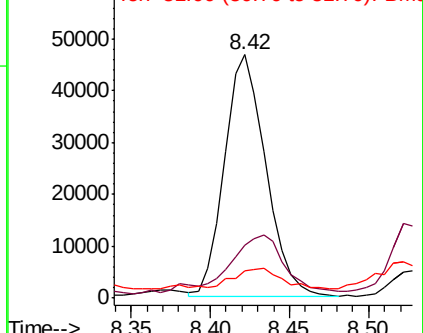

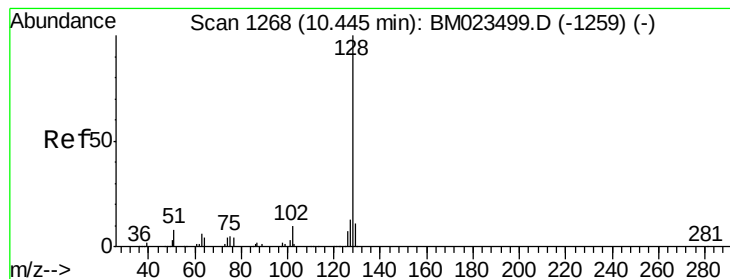

#28

Naphthalene

Concen: 63.037 ng/ul

RT: 10.45 min Scan# 1268

Delta R.T. -0.00 min

Lab File: BM023504.D

Acq: 31 Oct 2019 05:02

Instrument :

BNA_M

ClientSampleId :

BEJK8


Tgt Ion:128 Resp: 7673585

Ion Ratio Lower Upper

128 100

129 11.1 8.8 13.2

127 13.2 10.4 15.6



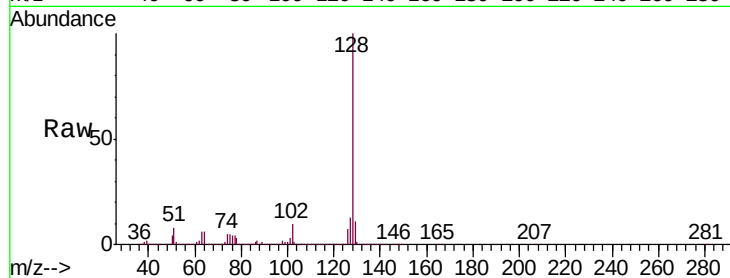


Abundance

Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

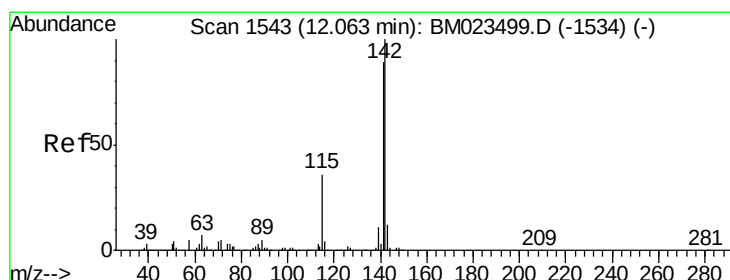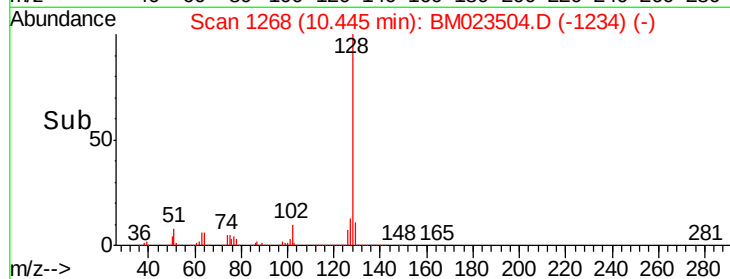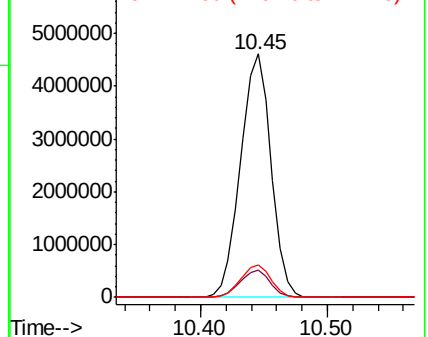

#34

2-Methylnaphthalene

Concen: 7.566 ng/ul

RT: 12.06 min Scan# 1543

Delta R.T. -0.00 min

Lab File: BM023504.D


Acq: 31 Oct 2019 05:02

Tgt Ion:142 Resp: 703589

Ion Ratio Lower Upper

142 100



141 88.1 72.4 108.6

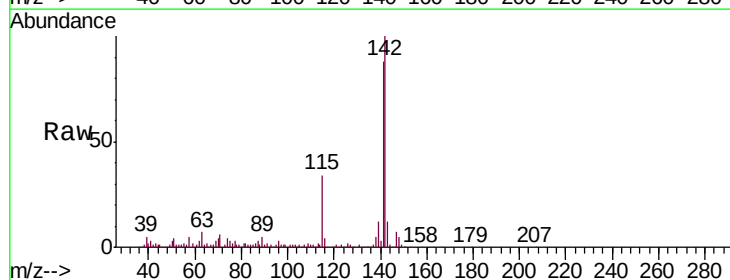


Abundance

Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

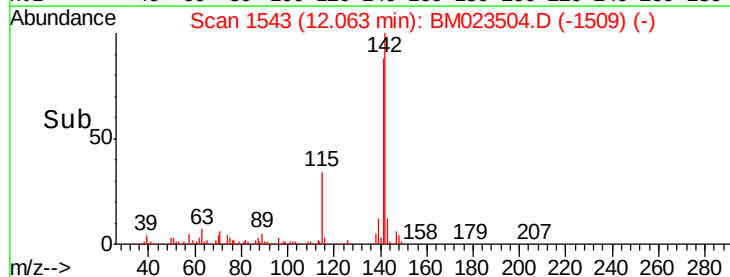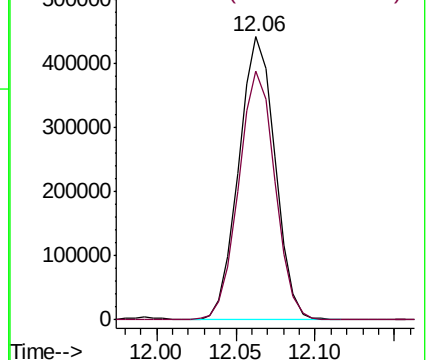

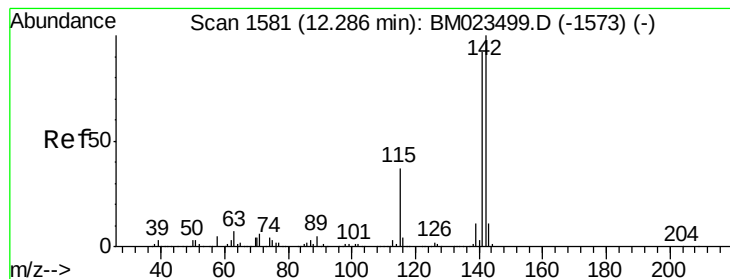

#35

1-Methylnaphthalene

Concen: 18.194 ng/ul

RT: 12.29 min Scan# 1581

Delta R.T. -0.00 min

Lab File: BM023504.D

Acq: 31 Oct 2019 05:02

Instrument :

BNA_M

ClientSampleId :

BEJK8


Tgt Ion:142 Resp: 1632615

Ion Ratio Lower Upper

142 100

141 93.2 73.6 110.4




116 3.9 3.3 4.9

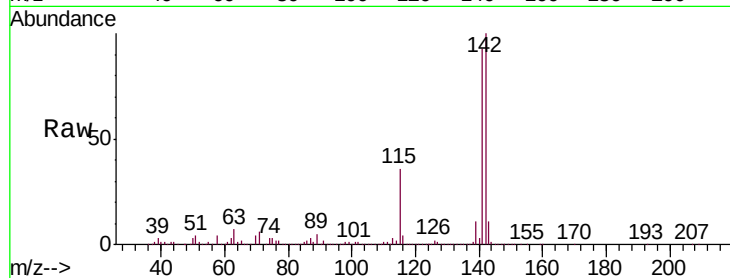

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

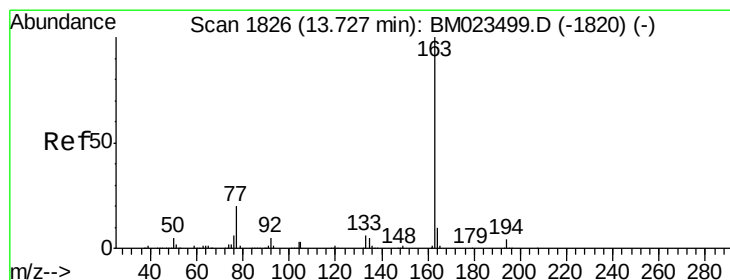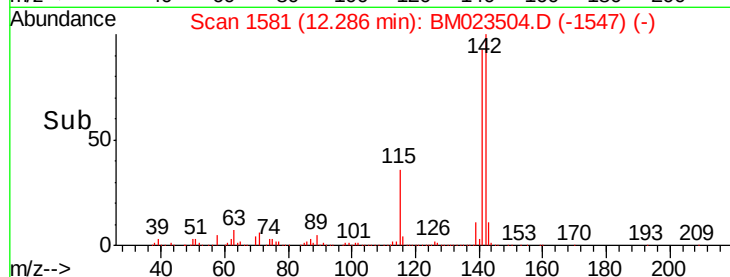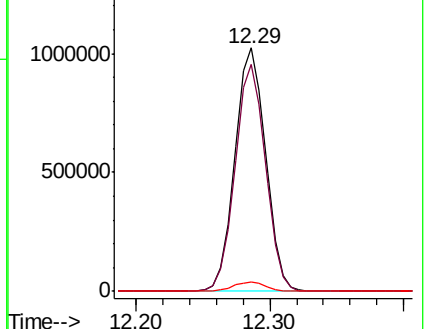

#45

Dimethylphthalate

Concen: 3.138 ng/ul

RT: 13.73 min Scan# 1826

Delta R.T. -0.00 min

Lab File: BM023504.D

Acq: 31 Oct 2019 05:02


Tgt Ion:163 Resp: 351031

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9



164 10.2 7.9 11.9

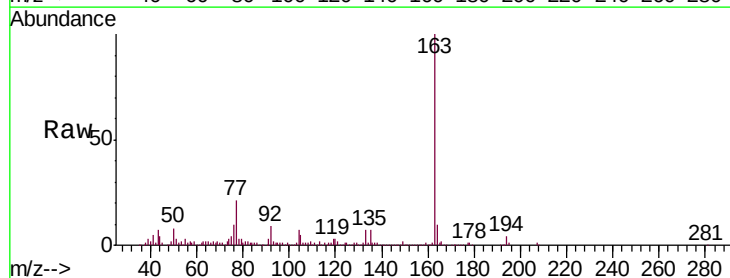


Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

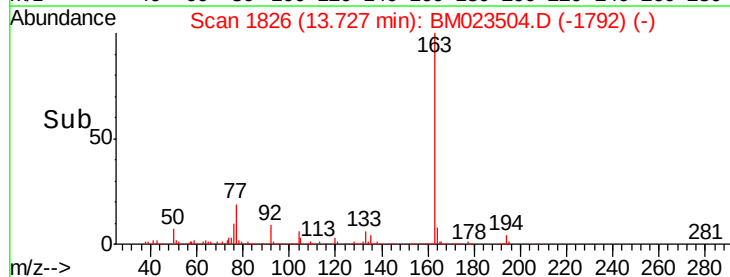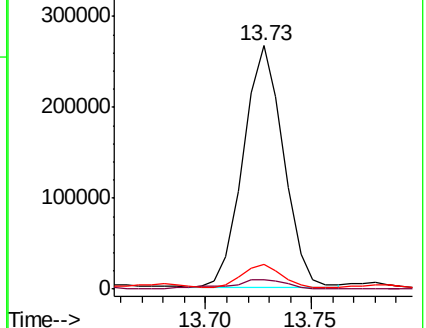

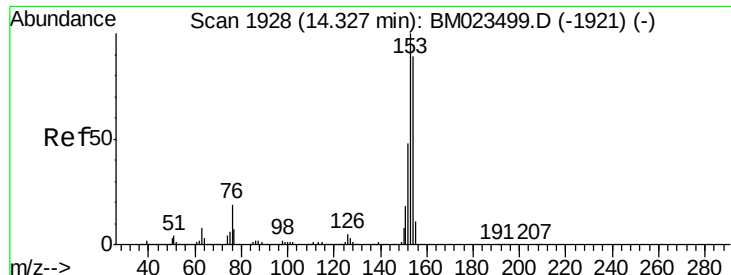

#50

Acenaphthene

Concen: 6.589 ng/ul

RT: 14.33 min Scan# 1928

Delta R.T. -0.00 min

Lab File: BM023504.D

Acq: 31 Oct 2019 05:02

Instrument :

BNA_M

ClientSampleId :

BEJK8


Tgt Ion:153 Resp: 613286

Ion Ratio Lower Upper

153 100

152 46.8 37.9 56.9

154 88.1 70.6 106.0

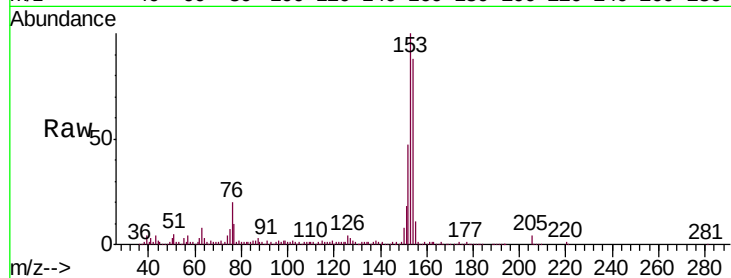

Abundance

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

