

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
 Data File : BM023517.D
 Acq On : 31 Oct 2019 12:50
 Operator : JU
 Sample : PB124083BL
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 31 15:24:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 31 06:46:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	401914	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1636270	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	994029	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.01	188	2100803	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1978562	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	2362823	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	52199	6.17	ng/uL	0.00
5) Phenol-d5	6.79	99	872851	25.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	568896	28.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	708562	26.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	664843	24.25	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	348609	28.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	368236	26.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	656498	24.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	105675	3.42	ng/ul	0.00
44) Dimethylphthalate-d6	13.68	166	2125919	28.16	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2404765	27.81	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	275949	21.10	ng/ul	0.00
58) Fluorene-d10	15.26	176	1816382	28.41	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	206788	15.81	ng/ul	0.00
71) Anthracene-d10	17.10	188	2708611	27.28	ng/ul	0.00
79) Pyrene-d10	19.41	212	2965970	27.26	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	3326329	27.63	ng/ul	0.00


Target Compounds				Ovalue	
46) 2,6-Dinitrotoluene	13.68	165	15210	1.013	ng/ul# 36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
Data File : BM023517.D
Acq On : 31 Oct 2019 12:50
Operator : JU
Sample : PB124083BL
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 31 15:24:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 31 06:46:10 2019
Response via : Initial Calibration

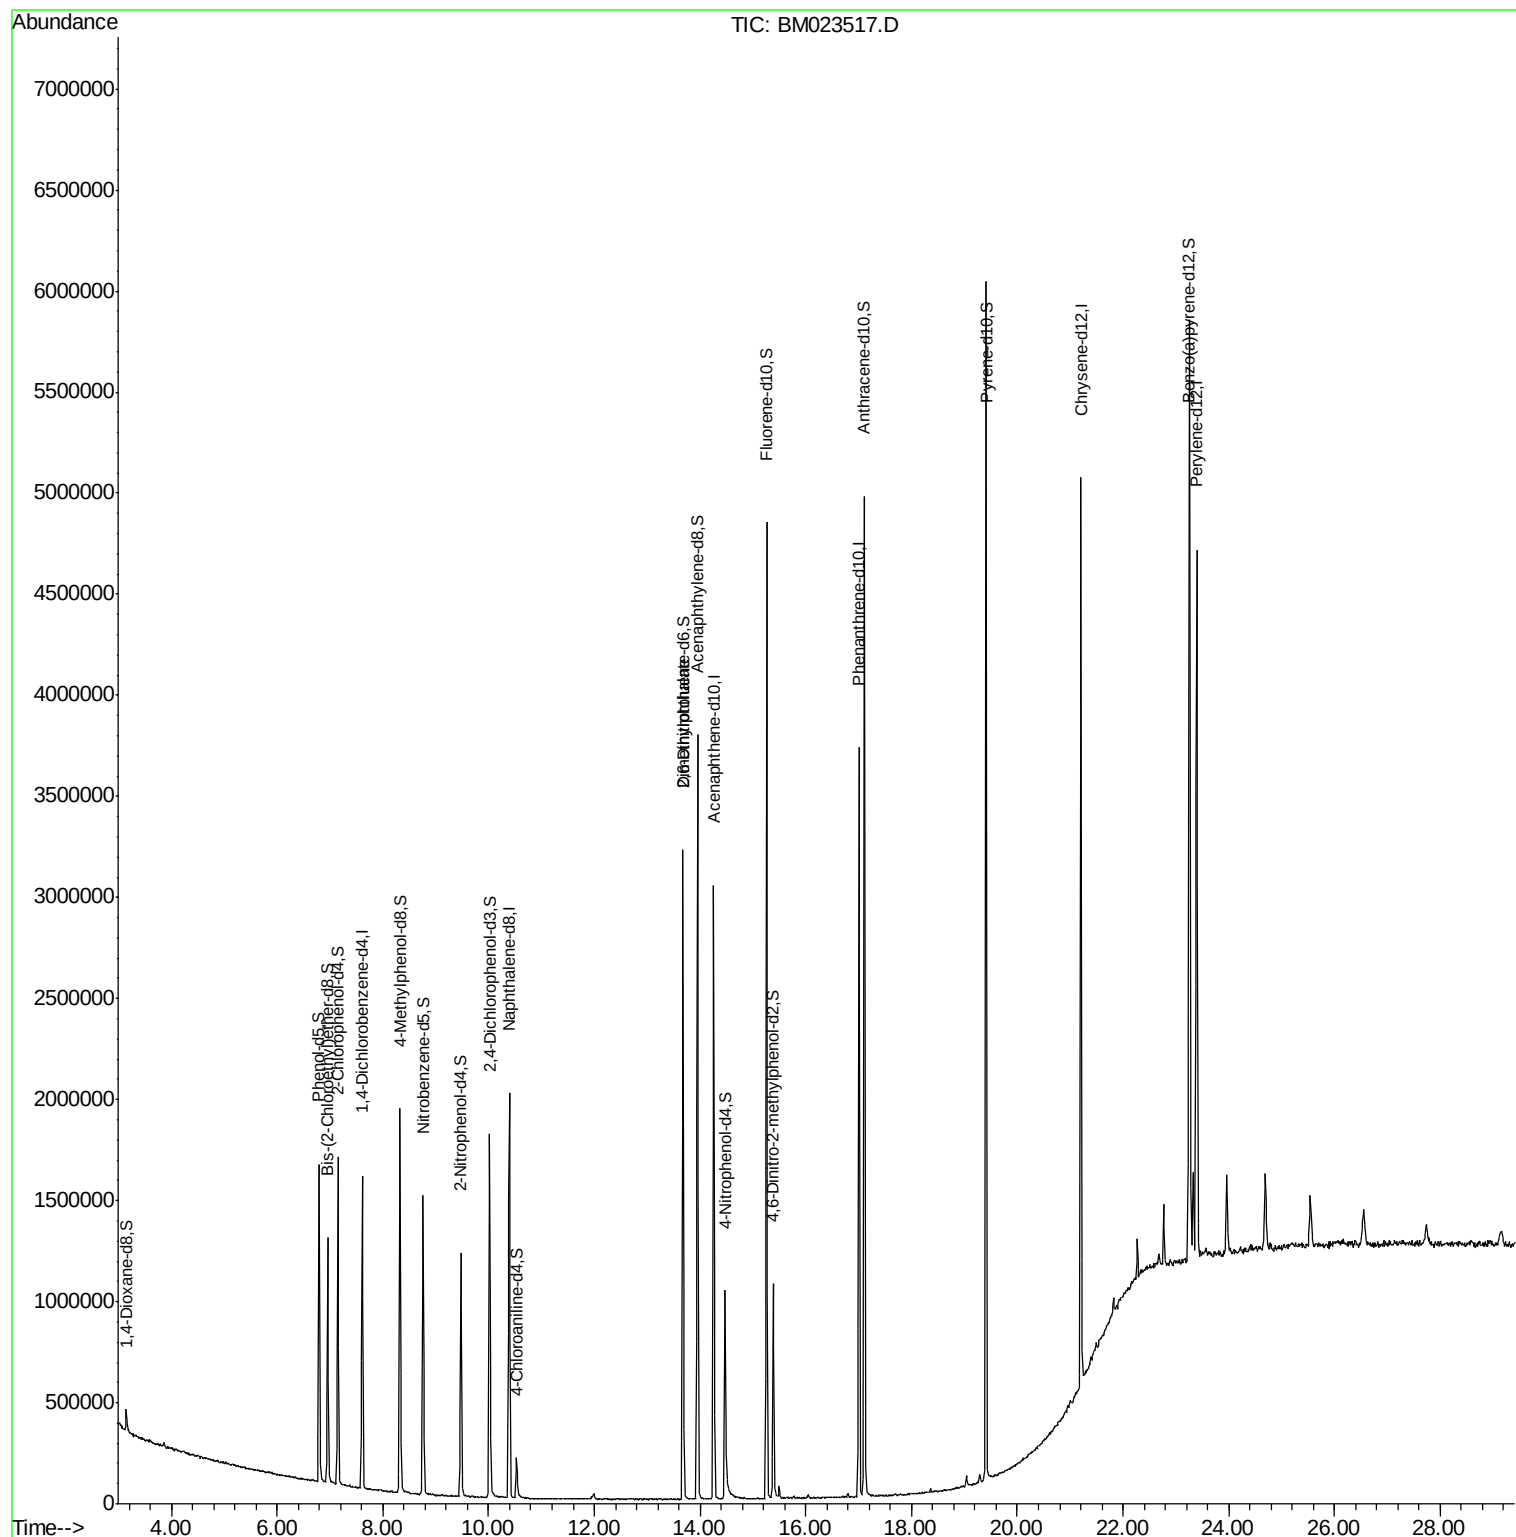

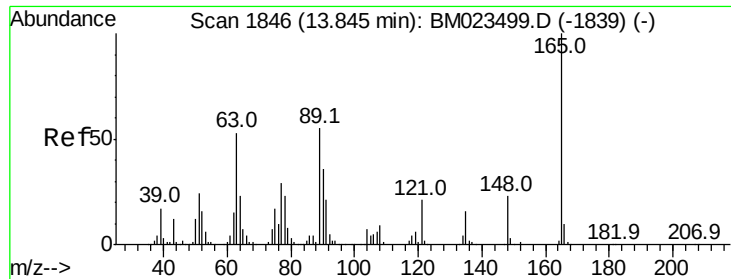

#46

2,6-Dinitrotoluene

Concen: 1.013 ng/ul

RT: 13.68 min Scan# 1818

Delta R.T. -0.16 min

Lab File: BM023517.D

Acq: 31 Oct 2019 12:50

Instrument :

BNA_M

ClientSampleId :


Tot Ion:165 Resp: 15210

Ion Ratio Lower Upper

165 100

89 0.0 44.3 66.5#

121 34.2 16.4 24.6#

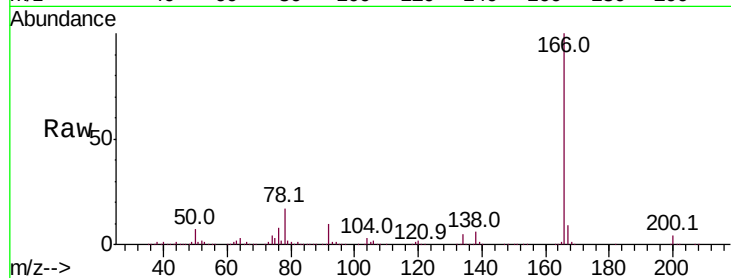

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

