

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
 Data File : BM023479.D
 Acq On : 30 Oct 2019 13:27
 Operator : JU
 Sample : K5434-06
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLNG7

Quant Time: Oct 30 17:14:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 25 07:44:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	391617	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.39	136	1589267	20.00	ng/ul	-0.03
36) Acenaphthene-d10	14.27	164	969904	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.02	188	1998637	20.00	ng/ul	-0.02
78) Chrysene-d12	21.21	240	2103597	20.00	ng/ul	-0.02
86) Perylene-d12	23.40	264	2498645	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	35351	4.29	ng/uL	0.00
5) Phenol-d5	6.80	99	722543	21.97	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	6.96	67	459414	23.83	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.16	132	592116	23.03	ng/ul	-0.02
13) 4-Methylphenol-d8	8.33	113	574994	21.52	ng/ul	-0.02
19) Nitrobenzene-d5	8.76	128	293539	24.53	ng/ul	-0.02
22) 2-Nitrophenol-d4	9.49	143	307602	23.17	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.02	165	553052	21.20	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.53	131	701489	23.39	ng/ul	-0.02
44) Dimethylphthalate-d6	13.69	166	1771296	24.05	ng/ul	-0.02
47) Acenaphthylene-d8	13.96	160	2047583	24.27	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.48	143	217363	17.04	ng/ul	-0.01
58) Fluorene-d10	15.26	176	1520036	24.37	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.39	200	178446	14.34	ng/ul	-0.02
71) Anthracene-d10	17.11	188	2407511	25.49	ng/ul	-0.02
79) Pyrene-d10	19.41	212	2839790	24.55	ng/ul	-0.02
90) Benzo(a)pyrene-d12	23.26	264	3442783	27.05	ng/ul	-0.02

Target Compounds


					Ovalue
6) Phenol	6.83	94	104888	3.097	ng/ul 99
45) Dimethylphthalate	13.73	163	936112	12.659	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
Data File : BM023479.D
Acq On : 30 Oct 2019 13:27
Operator : JU
Sample : K5434-06
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNG7

Quant Time: Oct 30 17:14:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 25 07:44:12 2019
Response via : Initial Calibration

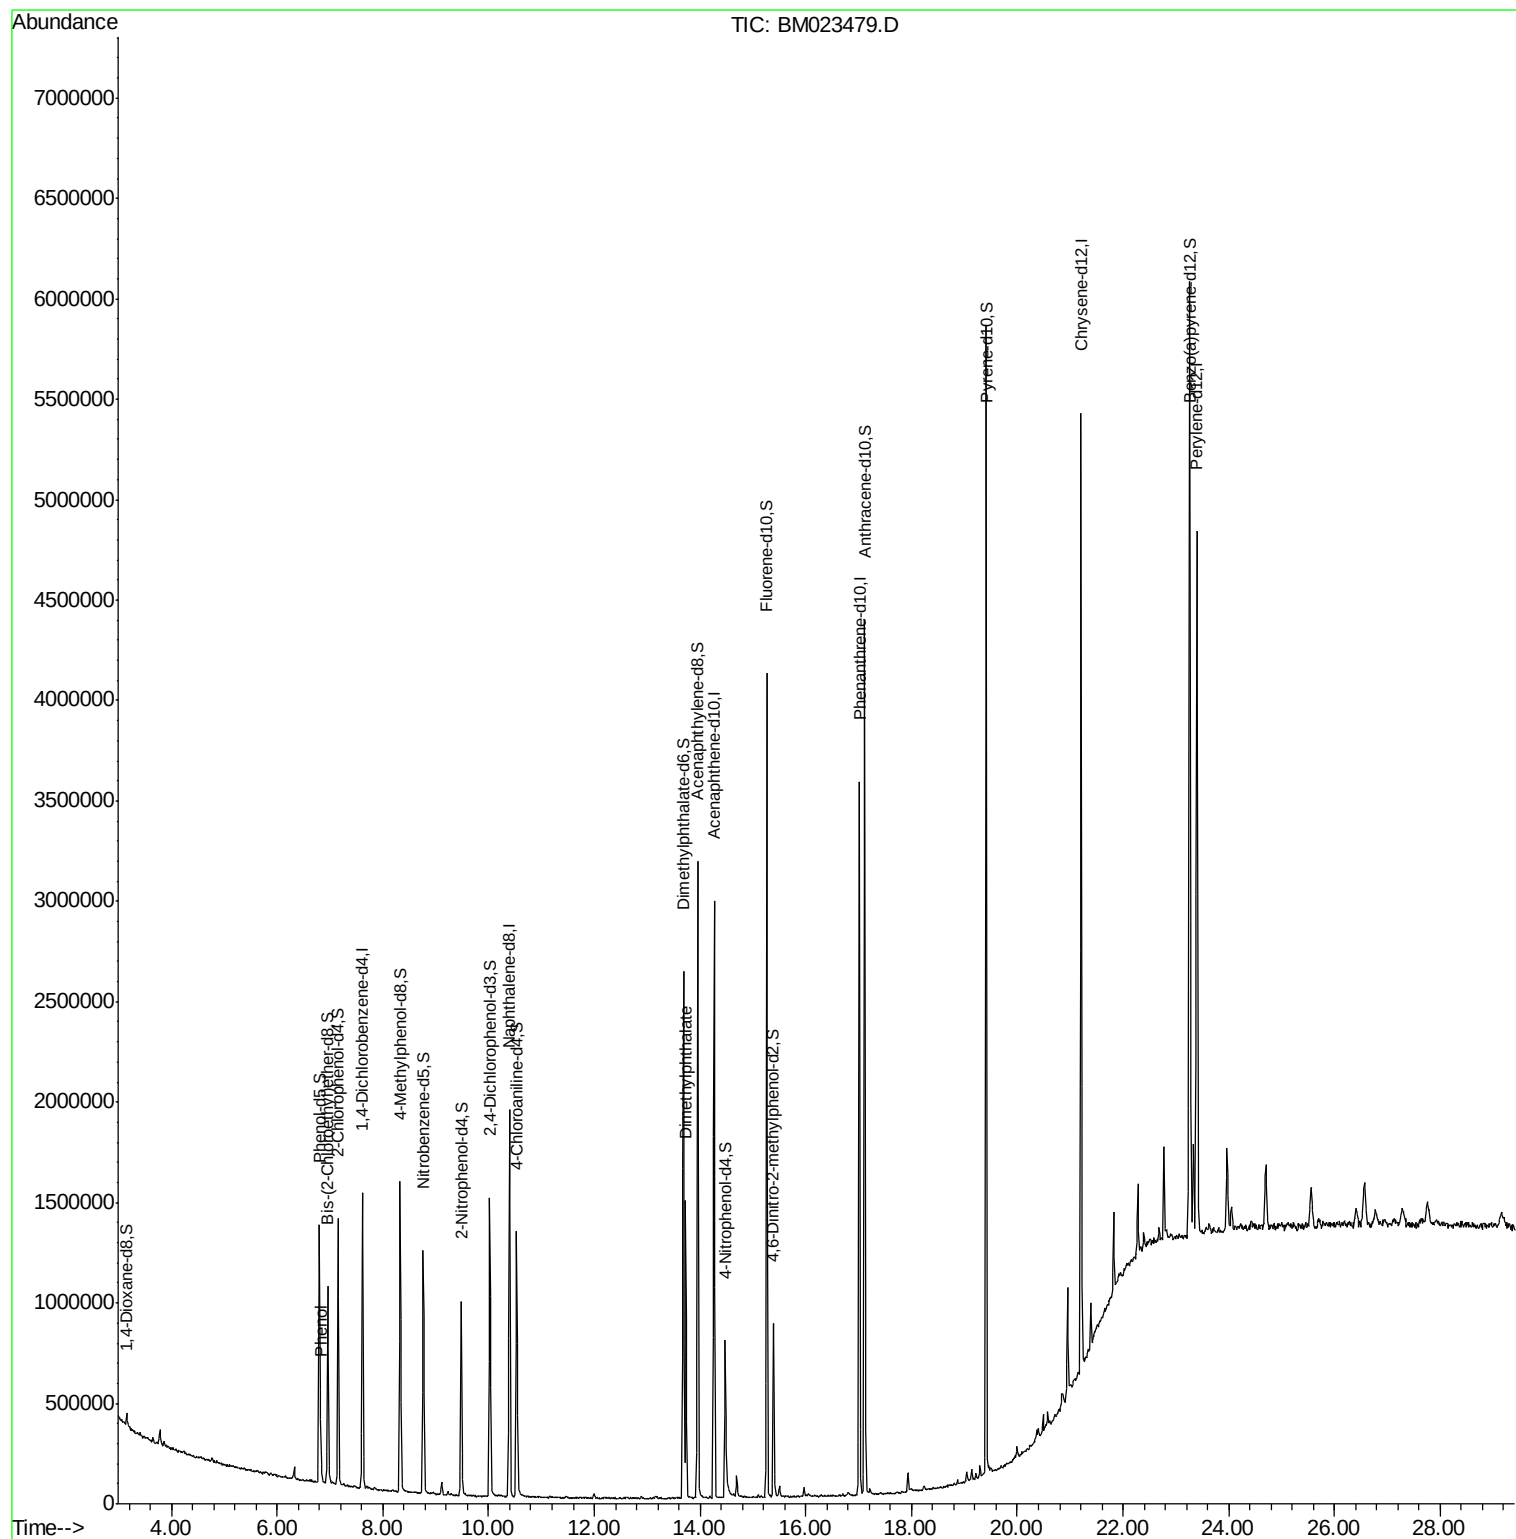

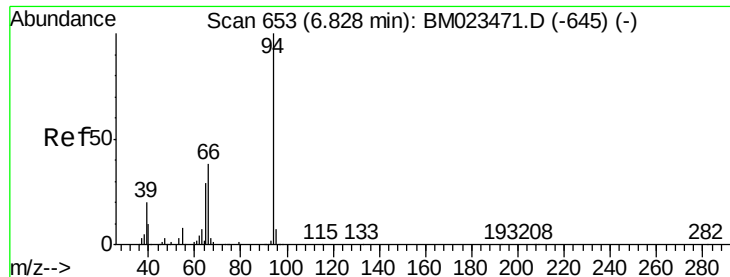

#6

Phenol

Concen: 3.097 ng/ul

RT: 6.83 min Scan# 653

Delta R.T. -0.02 min

Lab File: BM023479.D

Acq: 30 Oct 2019 13:27

Instrument :


BNA_M

ClientSampleId :

JLNG7

Tot Ion: 94 Resp: 104888

Ion	Ratio	Lower	Upper
94	100		
65	29.5	22.9	34.3
66	38.9	31.4	47.2



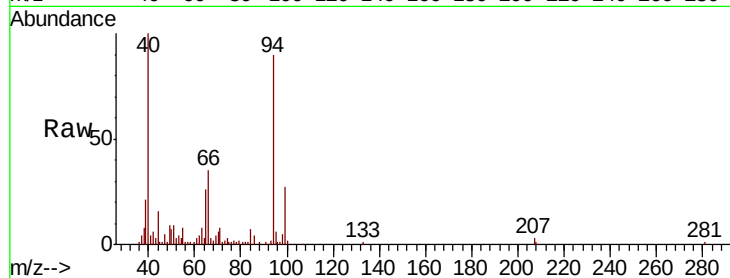


Abundance

Ion 94.00 (93.70 to 94.70): BM023471.D (-645) (-)

Ion 65.00 (64.70 to 65.70): BM023471.D (-645) (-)

Ion 66.00 (65.70 to 66.70): BM023471.D (-645) (-)

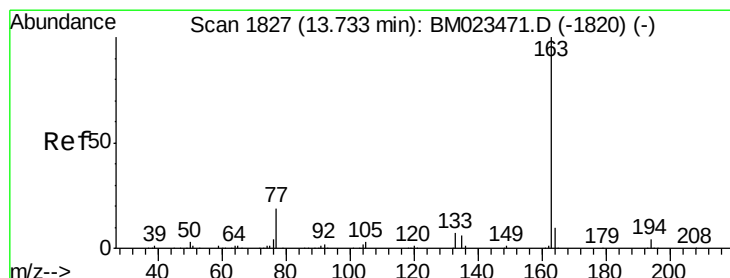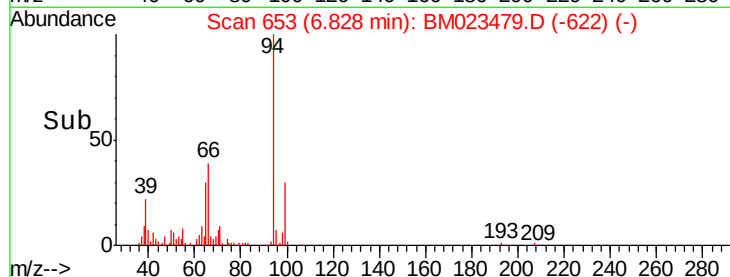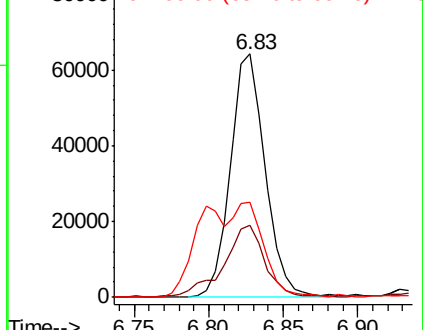

#45

Dimethylphthalate

Concen: 12.659 ng/ul

RT: 13.73 min Scan# 1826


Delta R.T. -0.03 min

Lab File: BM023479.D

Acq: 30 Oct 2019 13:27

Tgt Ion: 163 Resp: 936112

Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.3	4.9
164	10.5	7.9	11.9

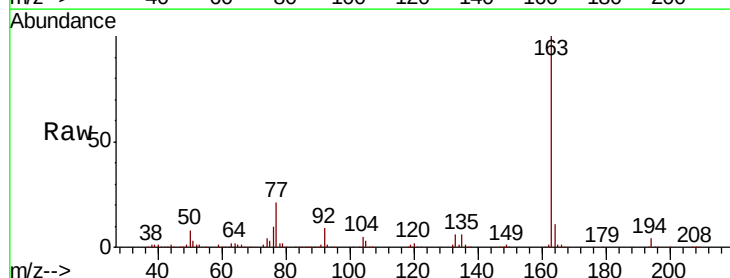

Abundance

Ion 163.00 (162.70 to 163.70): BM023471.D (-1820) (-)

Ion 194.00 (193.70 to 194.70): BM023471.D (-1820) (-)

Ion 164.00 (163.70 to 164.70): BM023471.D (-1820) (-)

