

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
 Data File : BM023489.D
 Acq On : 30 Oct 2019 19:27
 Operator : JU
 Sample : K5487-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE4H6

Quant Time: Oct 31 05:49:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 31 05:46:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	408157	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1672895	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	1034906	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.01	188	2119043	20.00	ng/ul	0.00
78) Chrysene-d12	21.21	240	2134777	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	2574635	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	45706	5.32	ng/uL	0.00
5) Phenol-d5	6.80	99	278720	8.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	652352	32.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	714741	26.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	488822	17.56	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	419188	33.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	450844	32.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	800261	29.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	56041	1.77	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	2788103	35.48	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	3127604	34.74	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	91448	6.72	ng/ul	0.00
58) Fluorene-d10	15.26	176	2313347	34.76	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	312142	23.66	ng/ul	0.00
71) Anthracene-d10	17.11	188	3676926	36.72	ng/ul	0.00
79) Pyrene-d10	19.41	212	4109769	35.01	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	4896848	37.34	ng/ul	0.00

Target Compounds


					Ovalue
45) Dimethylphthalate	13.73	163	306335	3.882	ng/ul 100
57) Diethylphthalate	15.10	149	103517	1.300	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
Data File : BM023489.D
Acq On : 30 Oct 2019 19:27
Operator : JU
Sample : K5487-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE4H6

Quant Time: Oct 31 05:49:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 31 05:46:17 2019
Response via : Initial Calibration

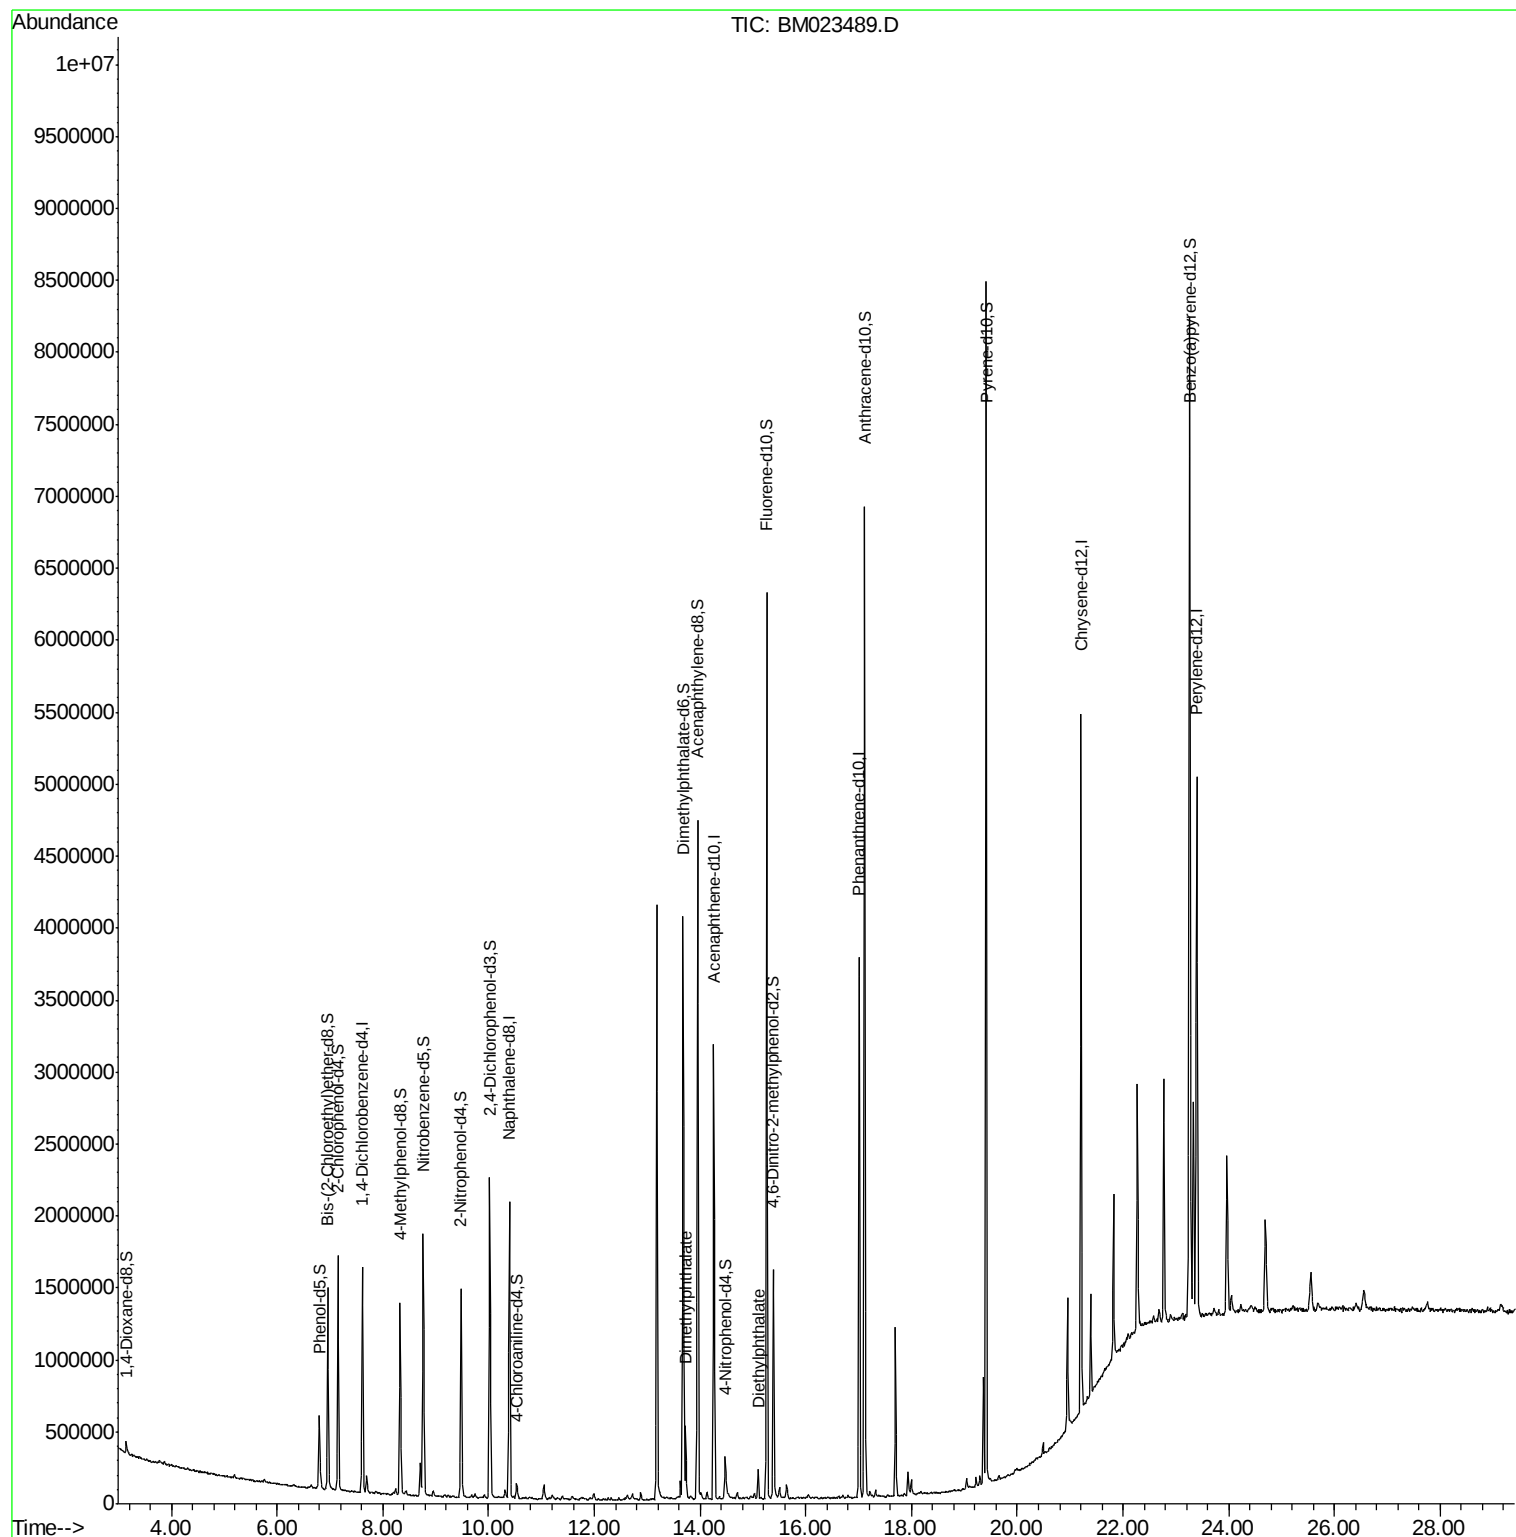

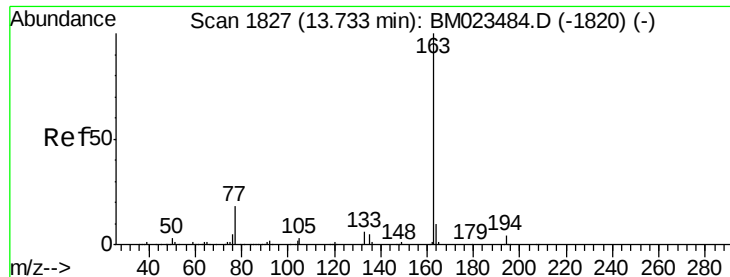

#45

Dimethylphthalate

Concen: 3.882 ng/ul

RT: 13.73 min Scan# 1826

Delta R.T. -0.01 min

Lab File: BM023489.D

Acq: 30 Oct 2019 19:27

Instrument :

BNA_M

ClientSampleId :

BE4H6


Tot Ion:163 Resp: 306335

Ion Ratio Lower Upper

163 100

194 4.5 3.3 4.9




164 9.8 7.9 11.9

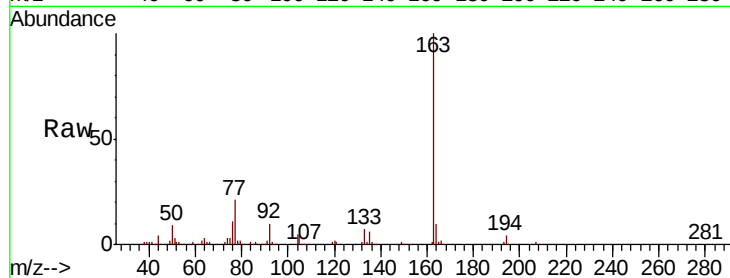

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

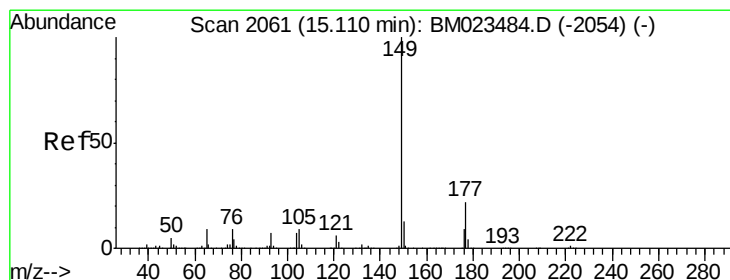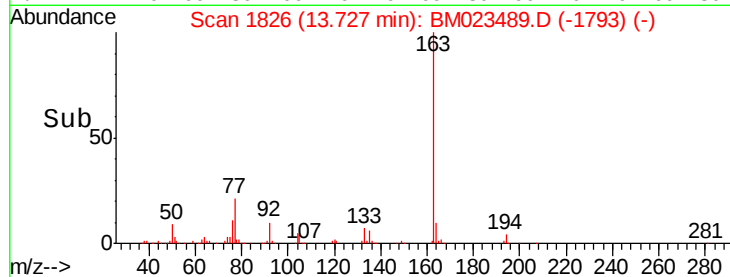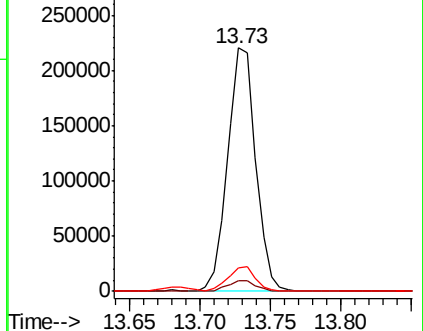

#57

Diethylphthalate

Concen: 1.300 ng/ul

RT: 15.10 min Scan# 2060

Delta R.T. -0.01 min

Lab File: BM023489.D

Acq: 30 Oct 2019 19:27


Tgt Ion:149 Resp: 103517

Ion Ratio Lower Upper

149 100

177 22.0 18.1 27.1

150 12.7 10.3 15.5

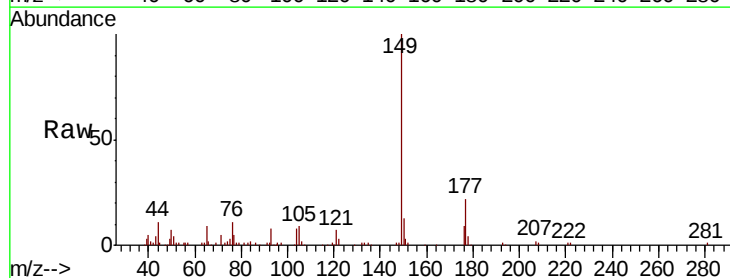

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 177.00 (176.70 to 177.70): E

Ion 150.00 (149.70 to 150.70): E

