

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
 Data File : BM023495.D
 Acq On : 30 Oct 2019 23:03
 Operator : JU
 Sample : K5487-07
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJJ9

Quant Time: Oct 31 05:49:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 31 05:46:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	496416	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1983514	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	1206344	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.01	188	2516564	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	2565903	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	3072609	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	52969	5.07	ng/uL	0.00
5) Phenol-d5	6.80	99	185993	4.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	551636	22.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	562771	17.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	353298	10.43	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	358716	24.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	377354	22.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	635019	19.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	43170	1.15	ng/ul	0.00
44) Dimethylphthalate-d6	13.68	166	2465387	26.91	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2697589	25.70	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	51740	3.26	ng/ul	0.00
58) Fluorene-d10	15.26	176	2005969	25.86	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	288769	18.43	ng/ul	0.00
71) Anthracene-d10	17.11	188	3350249	28.17	ng/ul	0.00
79) Pyrene-d10	19.41	212	3902576	27.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	4726447	30.20	ng/ul	-0.01


Target Compounds					Ovalue
45) Dimethylphthalate	13.73	163	147807	1.607	ng/ul 98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
Data File : BM023495.D
Acq On : 30 Oct 2019 23:03
Operator : JU
Sample : K5487-07
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJJ9

Quant Time: Oct 31 05:49:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 31 05:46:17 2019
Response via : Initial Calibration

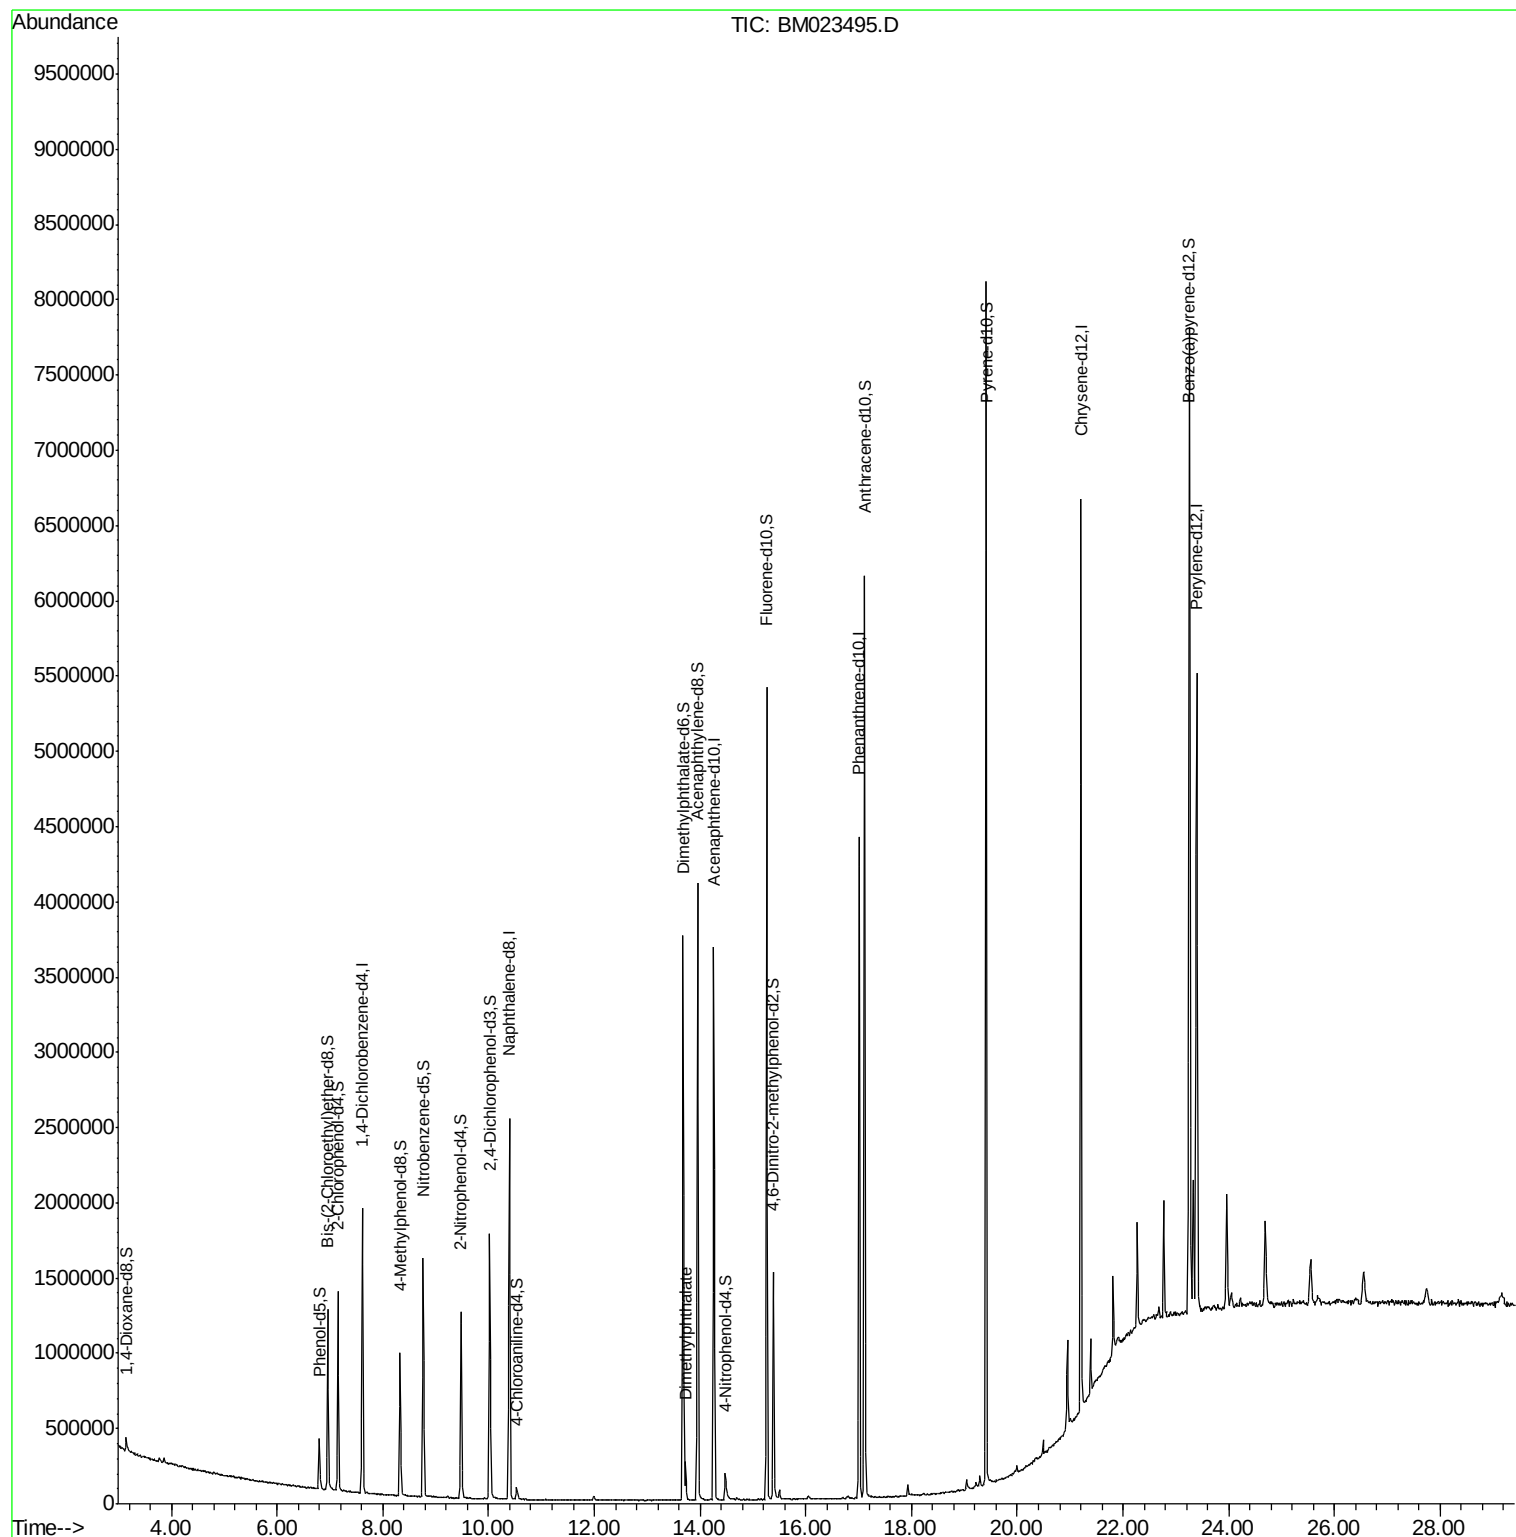

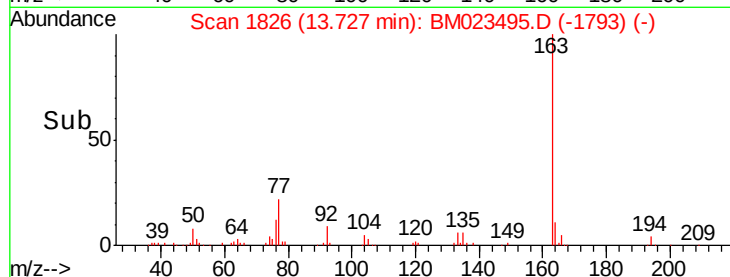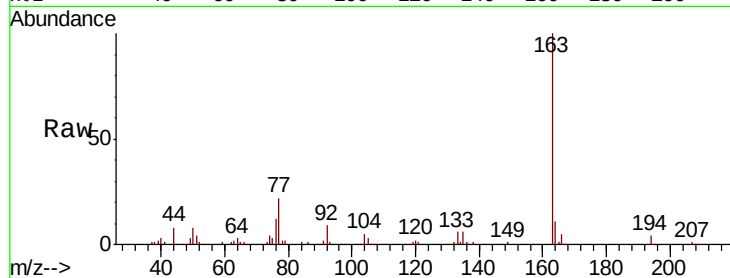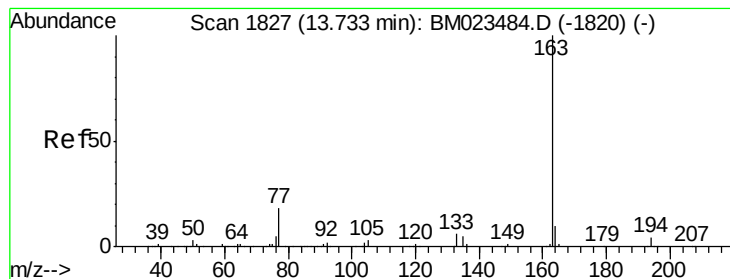

#45

Dimethylphthalate

Concen: 1.607 ng/ul

RT: 13.73 min Scan# 1826

Delta R.T. -0.01 min

Lab File: BM023495.D

Acq: 30 Oct 2019 23:03

Instrument :

BNA_M

ClientSampleId :

BEJJ9

Tot Ion:163 Resp: 147807

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.9 7.9 11.9

Abundance Ion 163.00 (162.70 to 163.70): E
150000 Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

