

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
 Data File : BM023501.D
 Acq On : 31 Oct 2019 03:14
 Operator : JU
 Sample : K5487-10
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJK5

Quant Time: Oct 31 06:48:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 31 06:46:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	504757	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1998632	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	1217487	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.01	188	2522892	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	2569647	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	3044006	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	59552	5.60	ng/uL	0.00
5) Phenol-d5	6.80	99	258822	6.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	632822	25.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	677368	20.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	449427	13.05	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	404170	26.86	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	426275	25.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	722986	22.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	44596	1.18	ng/ul	0.00
44) Dimethylphthalate-d6	13.68	166	2613982	28.27	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2895091	27.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	73371	4.58	ng/ul	0.00
58) Fluorene-d10	15.26	176	2197012	28.06	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	314272	20.01	ng/ul	0.00
71) Anthracene-d10	17.11	188	3604227	30.23	ng/ul	0.00
79) Pyrene-d10	19.41	212	4052638	28.68	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	4845932	31.25	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.73	163	318765	3.434	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
Data File : BM023501.D
Acq On : 31 Oct 2019 03:14
Operator : JU
Sample : K5487-10
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJK5

Quant Time: Oct 31 06:48:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 31 06:46:10 2019
Response via : Initial Calibration

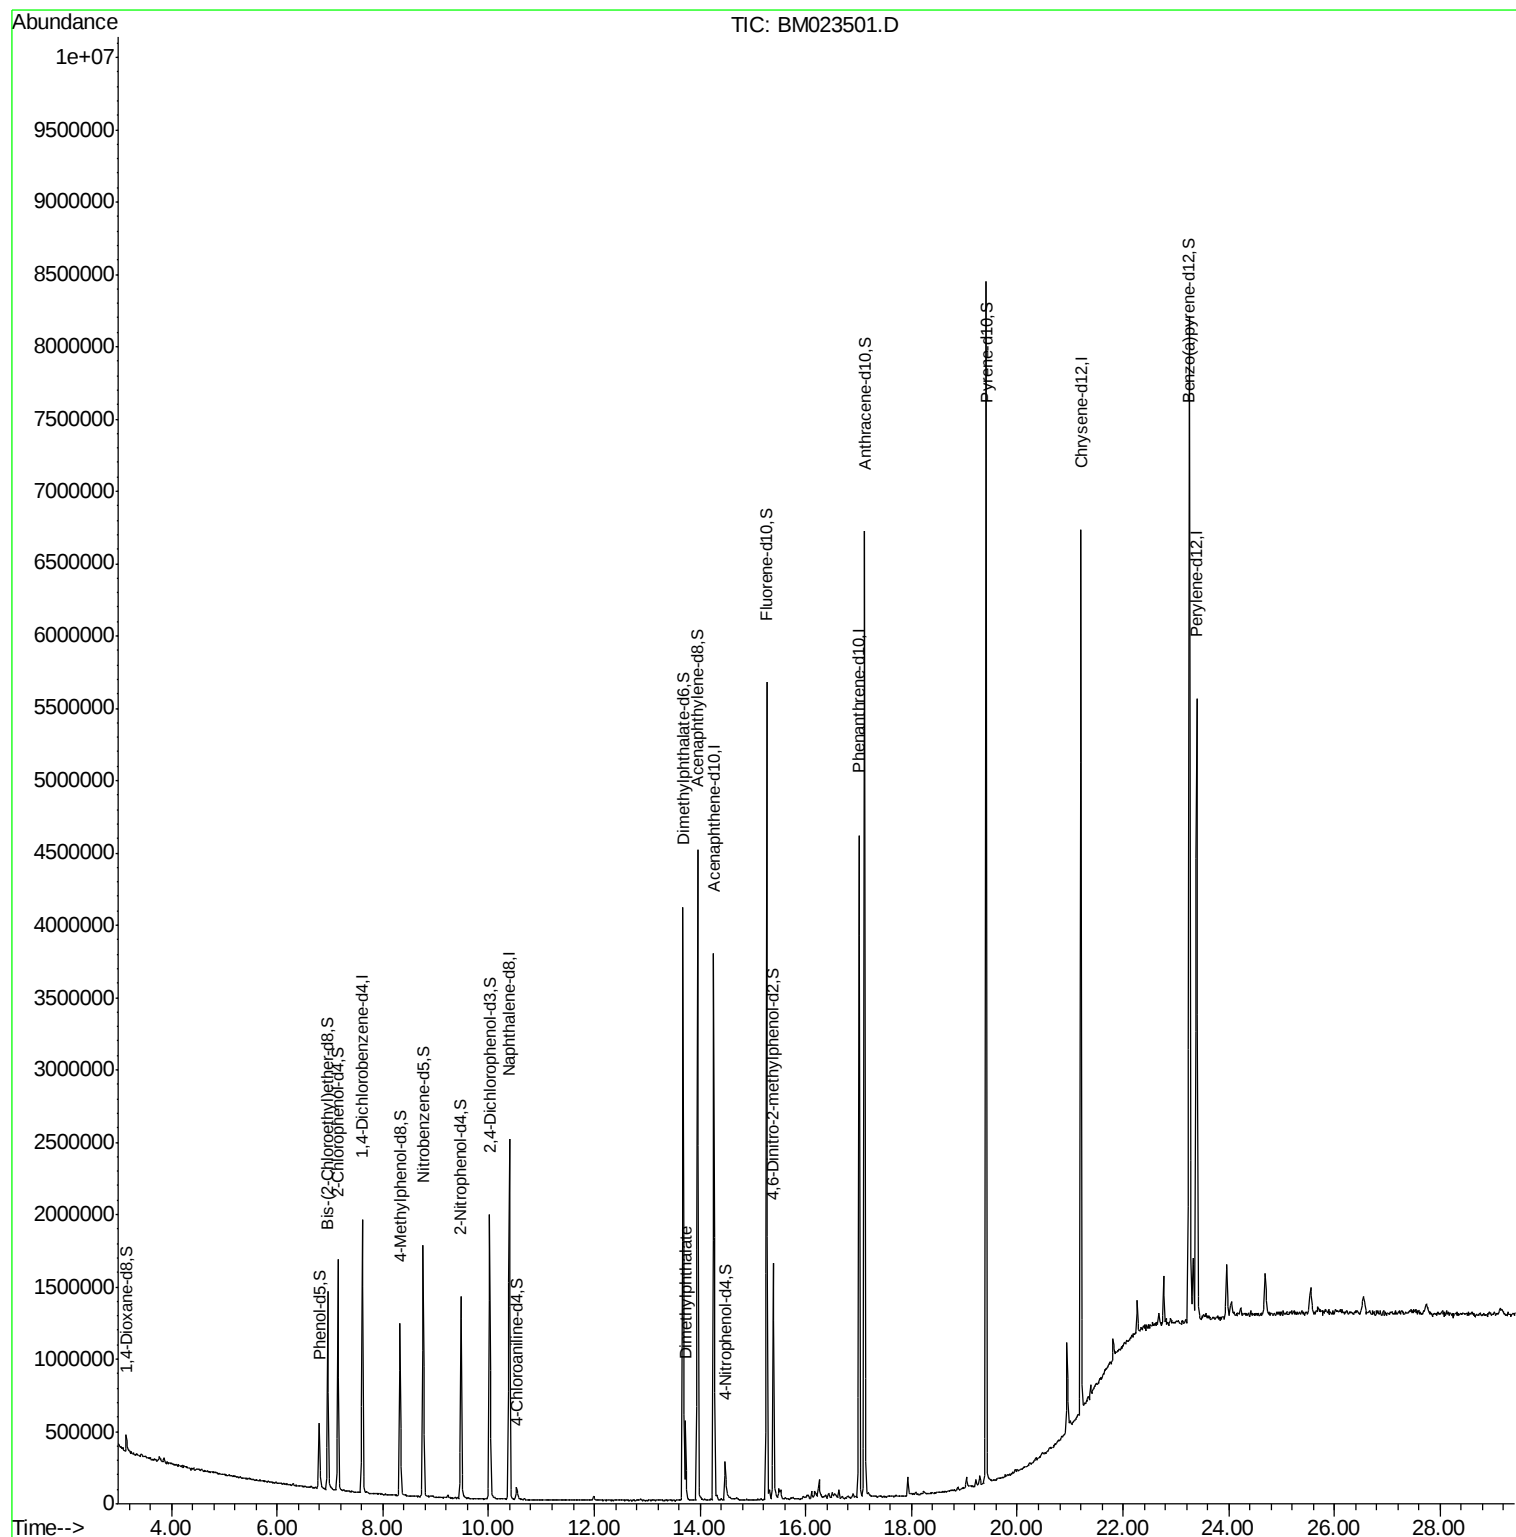

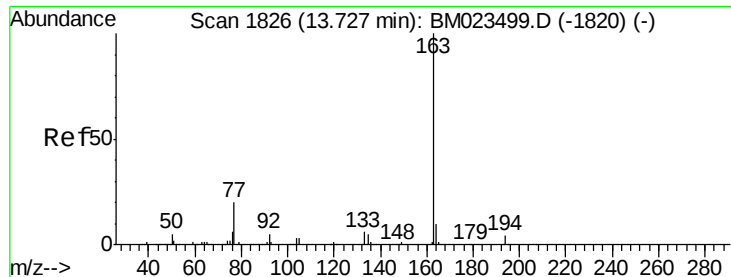

#45

Dimethylphthalate

Concen: 3.434 ng/ul

RT: 13.73 min Scan# 1826

Delta R.T. 0.00 min

Lab File: BM023501.D

Acq: 31 Oct 2019 03:14

Instrument :

BNA_M

ClientSampleId :

BEJK5


Tot Ion:163 Resp: 318765

Ion Ratio Lower Upper

163 100

194 4.4 3.3 4.9

164 9.7 7.9 11.9

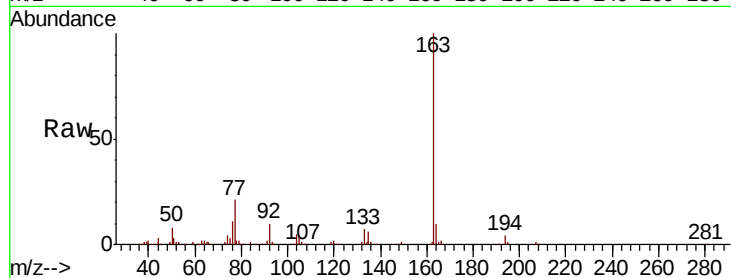

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

