

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
 Data File : BM023503.D
 Acq On : 31 Oct 2019 04:26
 Operator : JU
 Sample : K5487-12
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJK7

Quant Time: Oct 31 06:48:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 31 06:46:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	520861	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	2069551	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	1255948	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.01	188	2582180	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	2675719	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	3158381	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	54071	4.93	ng/uL	0.00
5) Phenol-d5	6.79	99	200978	4.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	517455	20.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	555512	16.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	360647	10.15	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	330939	21.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	349039	20.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	611751	18.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	39501	1.01	ng/ul	0.00
44) Dimethylphthalate-d6	13.68	166	2233479	23.42	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2394854	21.92	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	65772	3.98	ng/ul	0.00
58) Fluorene-d10	15.26	176	1872488	23.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	279598	17.39	ng/ul	0.00
71) Anthracene-d10	17.11	188	3238265	26.54	ng/ul	0.00
79) Pyrene-d10	19.41	212	3702212	25.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	4393981	27.31	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.73	163	377151	3.938	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
Data File : BM023503.D
Acq On : 31 Oct 2019 04:26
Operator : JU
Sample : K5487-12
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJK7

Quant Time: Oct 31 06:48:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 31 06:46:10 2019
Response via : Initial Calibration

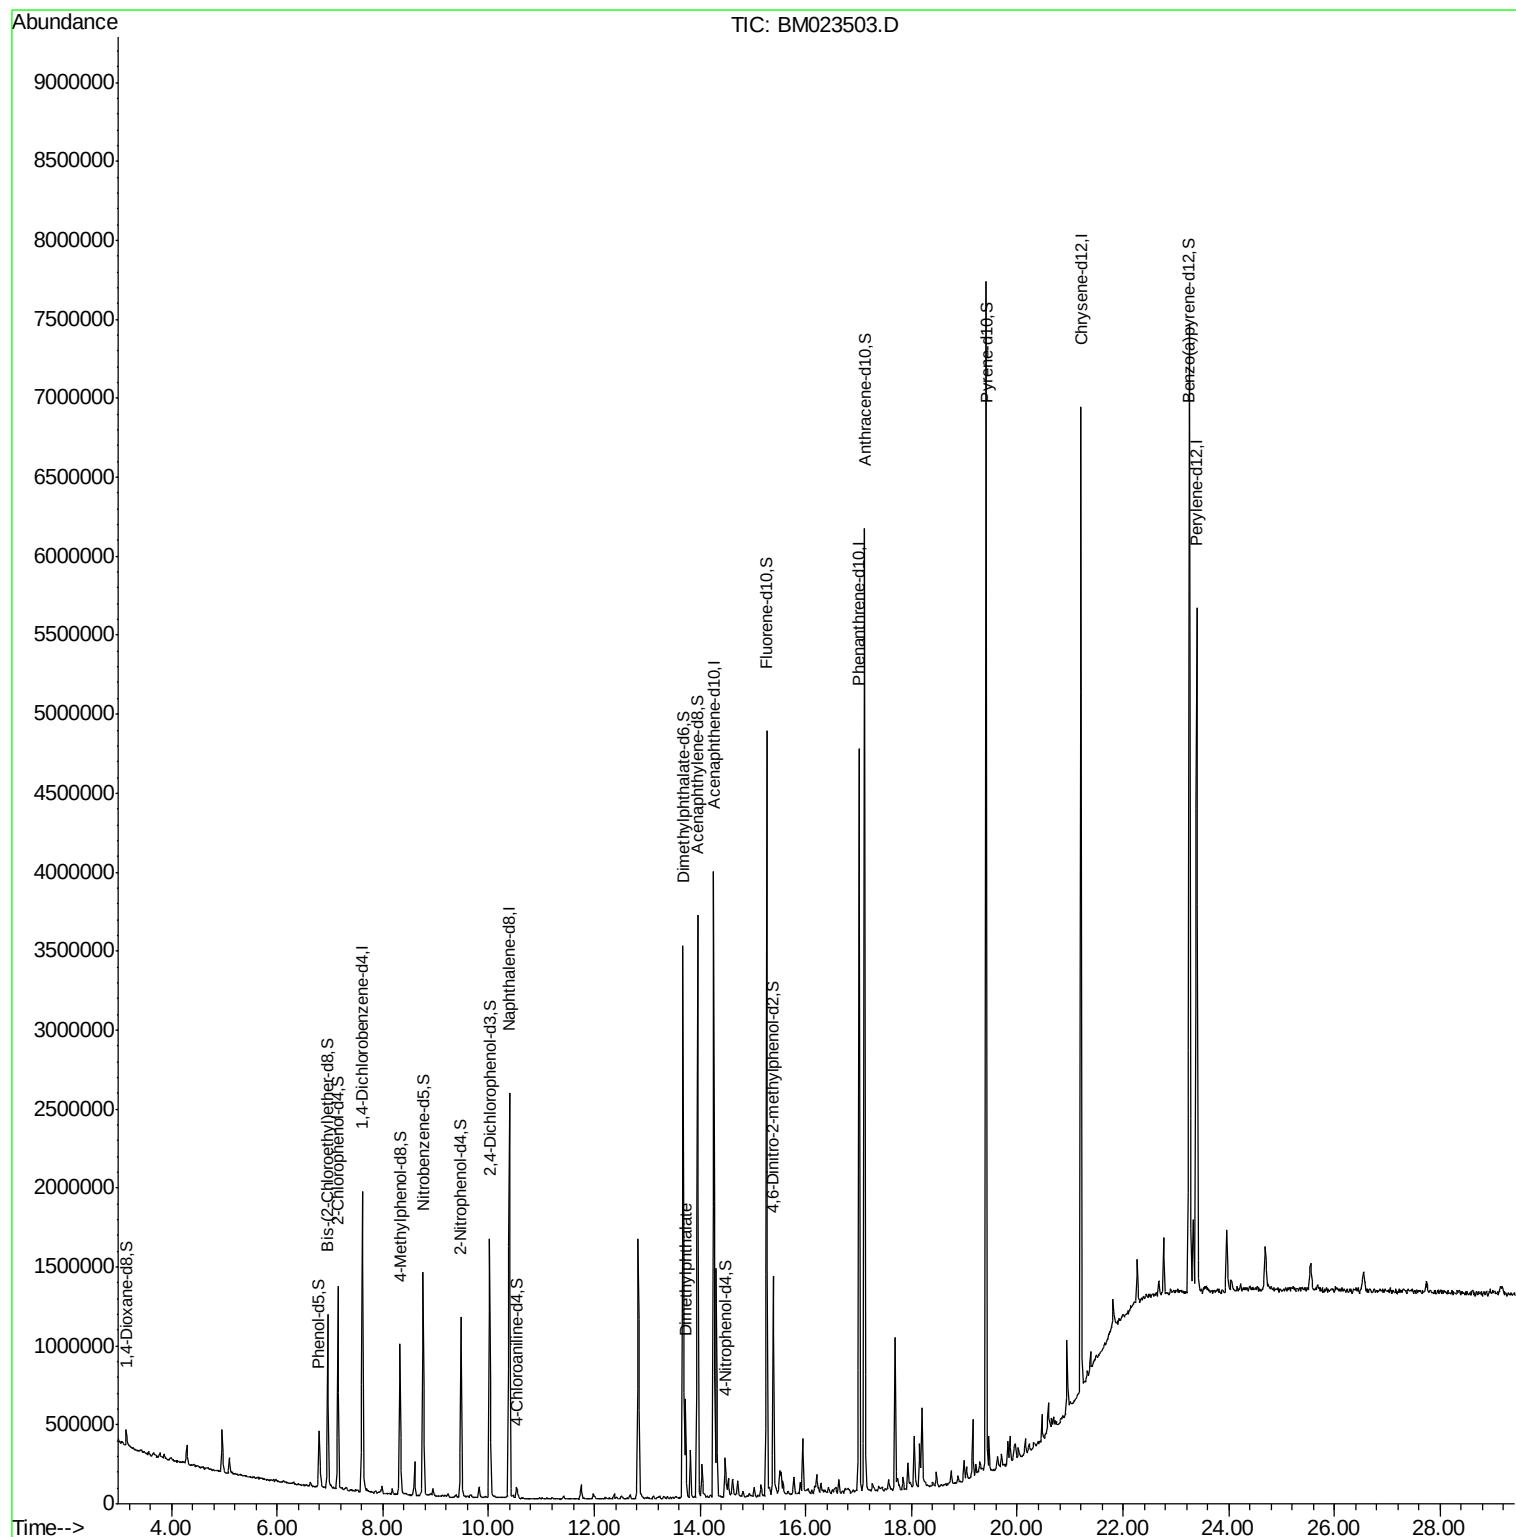

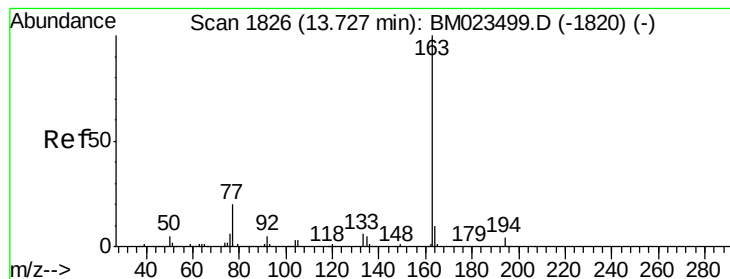

#45

Dimethylphthalate

Concen: 3.938 ng/ul

RT: 13.73 min Scan# 1826

Delta R.T. 0.00 min

Lab File: BM023503.D

Acq: 31 Oct 2019 04:26

Instrument :

BNA_M

ClientSampleId :

BEJK7



Tot Ion:163 Resp: 377151

Ion Ratio Lower Upper

163 100

194 4.3 3.3 4.9

164 10.7 7.9 11.9

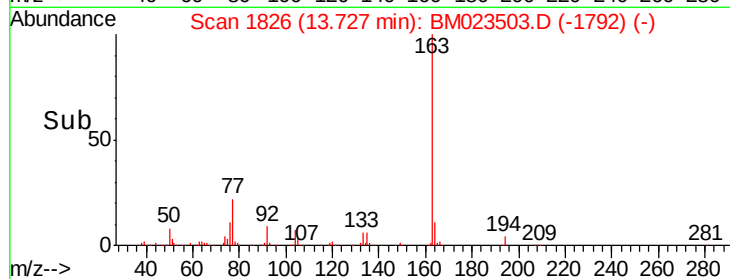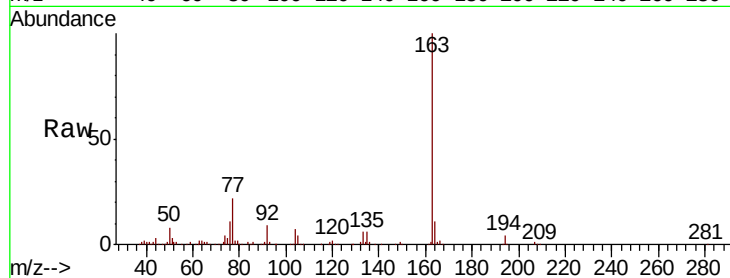

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

