

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
 Data File : BM023510.D
 Acq On : 31 Oct 2019 08:38
 Operator : JU
 Sample : K5487-19
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJL4

Quant Time: Oct 31 10:29:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 31 06:46:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	595132	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	2395726	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	1438235	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.01	188	2995891	20.00	ng/ul	0.00
78) Chrysene-d12	21.21	240	3049388	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	3214152	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	106440	8.50	ng/uL	0.00
5) Phenol-d5	6.80	99	262825	5.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	599054	20.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	671319	17.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	468233	11.53	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	405282	22.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	441204	22.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	799453	20.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	60368	1.34	ng/ul	0.00
44) Dimethylphthalate-d6	13.68	166	2709286	24.81	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	3080598	24.62	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	86714	4.58	ng/ul	0.00
58) Fluorene-d10	15.26	176	2308751	24.96	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	334249	17.92	ng/ul	0.00
71) Anthracene-d10	17.11	188	3672558	25.94	ng/ul	0.00
79) Pyrene-d10	19.41	212	4126766	24.61	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	4873855	29.77	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	345837	3.154	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM102919\
Data File : BM023510.D
Acq On : 31 Oct 2019 08:38
Operator : JU
Sample : K5487-19
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJL4

Quant Time: Oct 31 10:29:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 31 06:46:10 2019
Response via : Initial Calibration

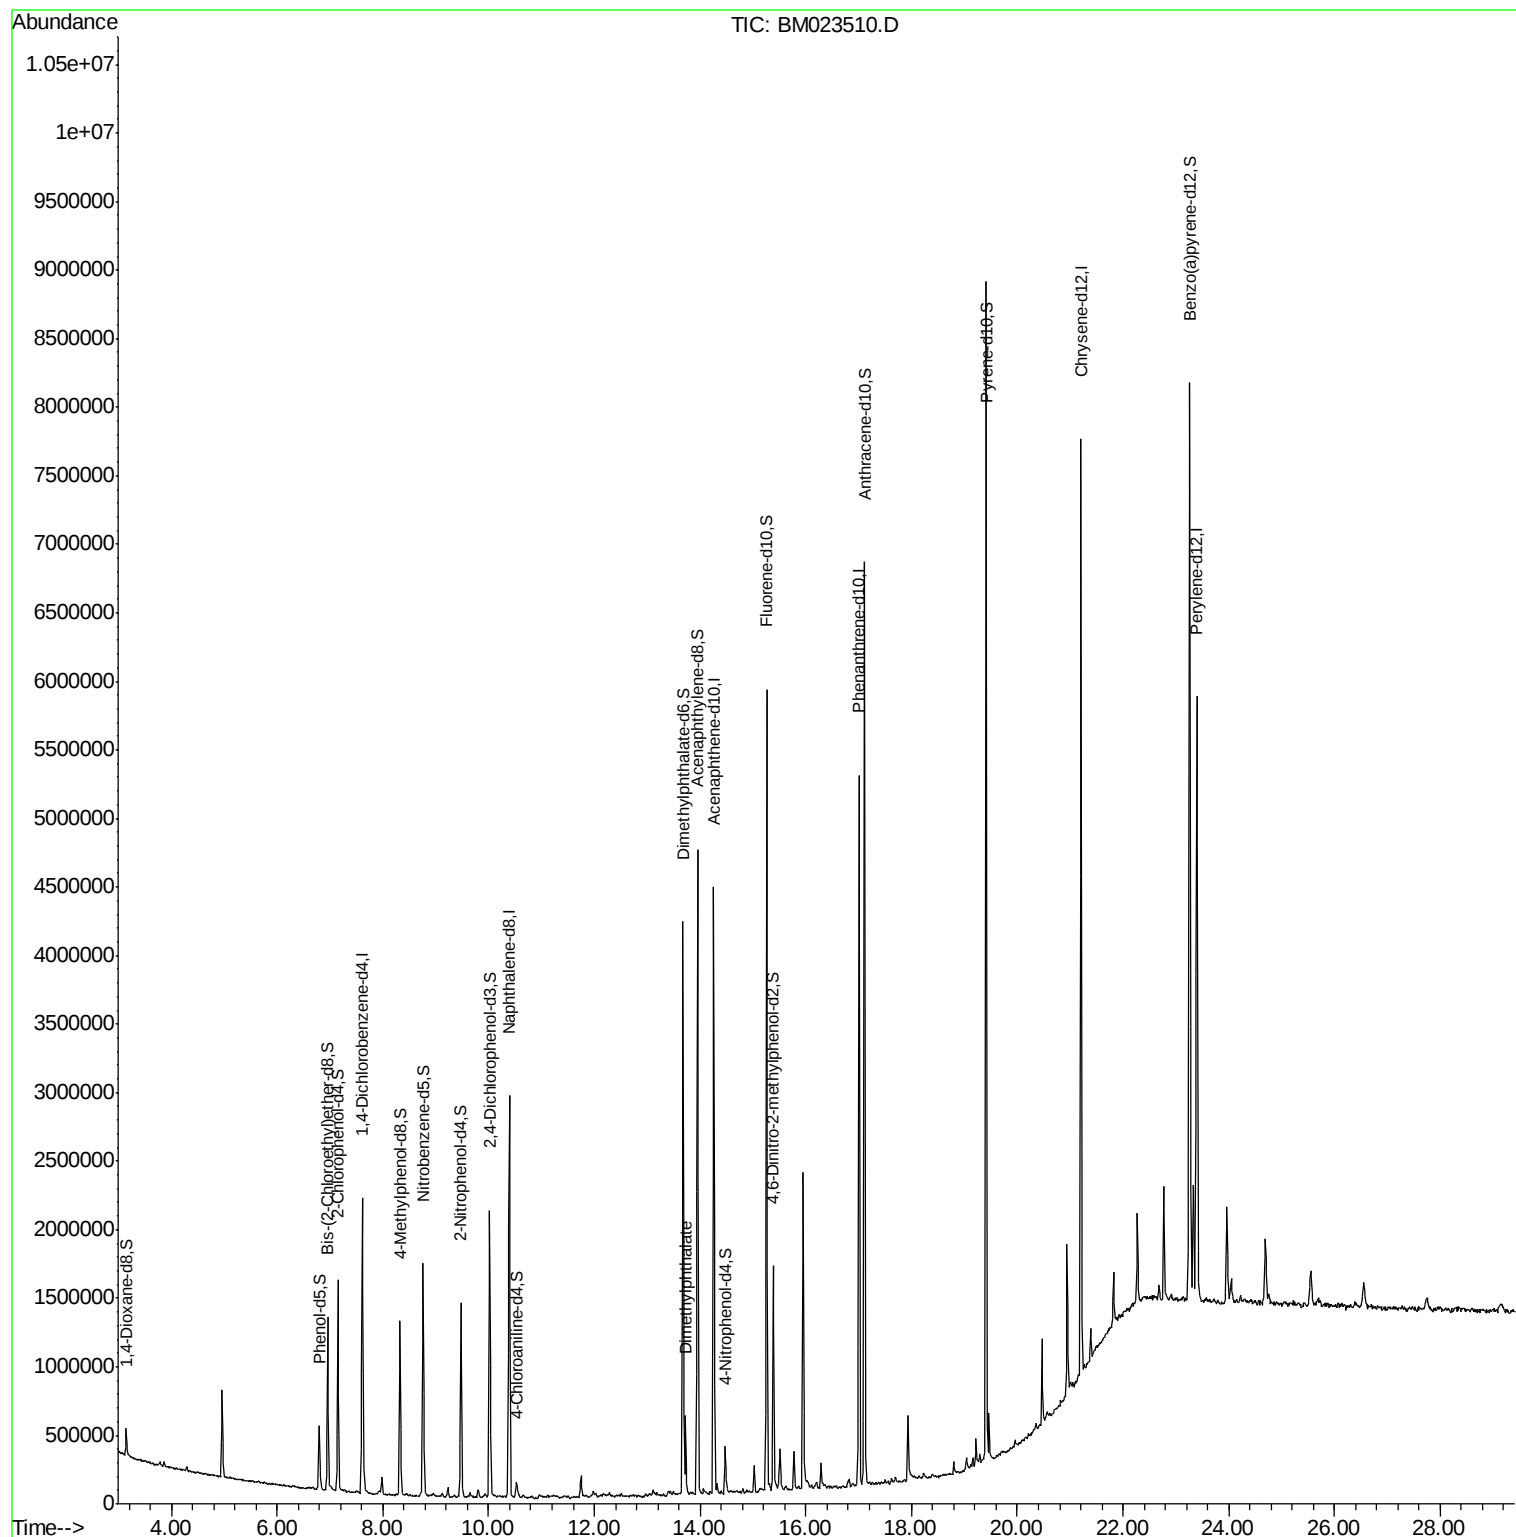

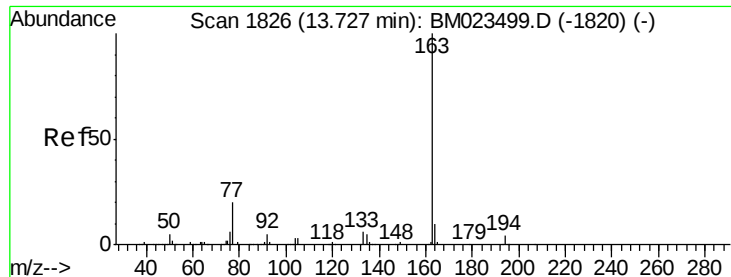

#45

Dimethylphthalate

Concen: 3.154 ng/ul

RT: 13.73 min Scan# 1826

Delta R.T. 0.00 min

Lab File: BM023510.D

Acq: 31 Oct 2019 08:38

Instrument :

BNA_M

ClientSampleId :

BEJL4


Tot Ion:163 Resp: 345837

Ion Ratio Lower Upper

163 100

194 4.6 3.3 4.9

164 9.7 7.9 11.9

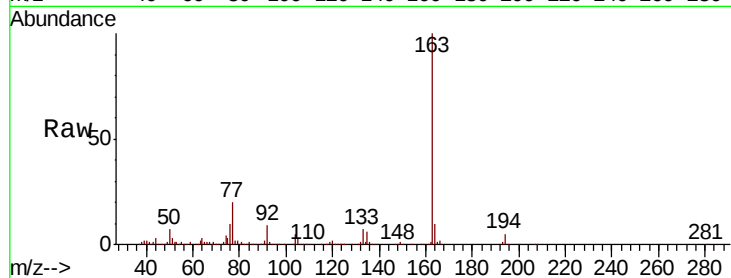

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

