

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
 Data File : BM012570.D
 Acq On : 30 Oct 2017 13:16
 Operator : SJ/JU
 Sample : I6045-02
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 31 03:00:37 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 31 03:00:36 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	326261	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	1233469	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	697096	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.23	188	1573728	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1838678	20.00	ng/ul	0.00
83) Perylene-d12	23.70	264	2079693	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.35	96	50865	7.96	ng/uL	0.00
5) Phenol-d5	7.03	99	890665	32.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.19	67	539969	33.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.39	132	720644	35.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.56	113	730949	31.38	ng/ul	0.00
19) Nitrobenzene-d5	9.02	128	342814	44.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	392160	49.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	724258	34.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.79	131	876633	39.44	ng/ul	0.00
43) Dimethylphthalate-d6	13.90	166	2041517	33.52	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	2602137	36.12	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	343848	37.98	ng/ul	0.00
57) Fluorene-d10	15.49	176	1745865	33.87	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.60	200	274897	36.09	ng/ul	0.00
70) Anthracene-d10	17.33	188	2700386	36.01	ng/ul	0.00
76) Pyrene-d10	19.62	212	3006929	35.65	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	3517667	35.60	ng/ul	0.00


Target Compounds					Ovalue
45) 2,6-Dinitrotoluene	13.90	165	15616	1.63	ng/ul# 28


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
Data File : BM012570.D
Acq On : 30 Oct 2017 13:16
Operator : SJ/JU
Sample : I6045-02
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 31 03:00:37 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 31 03:00:36 2017
Response via : Initial Calibration

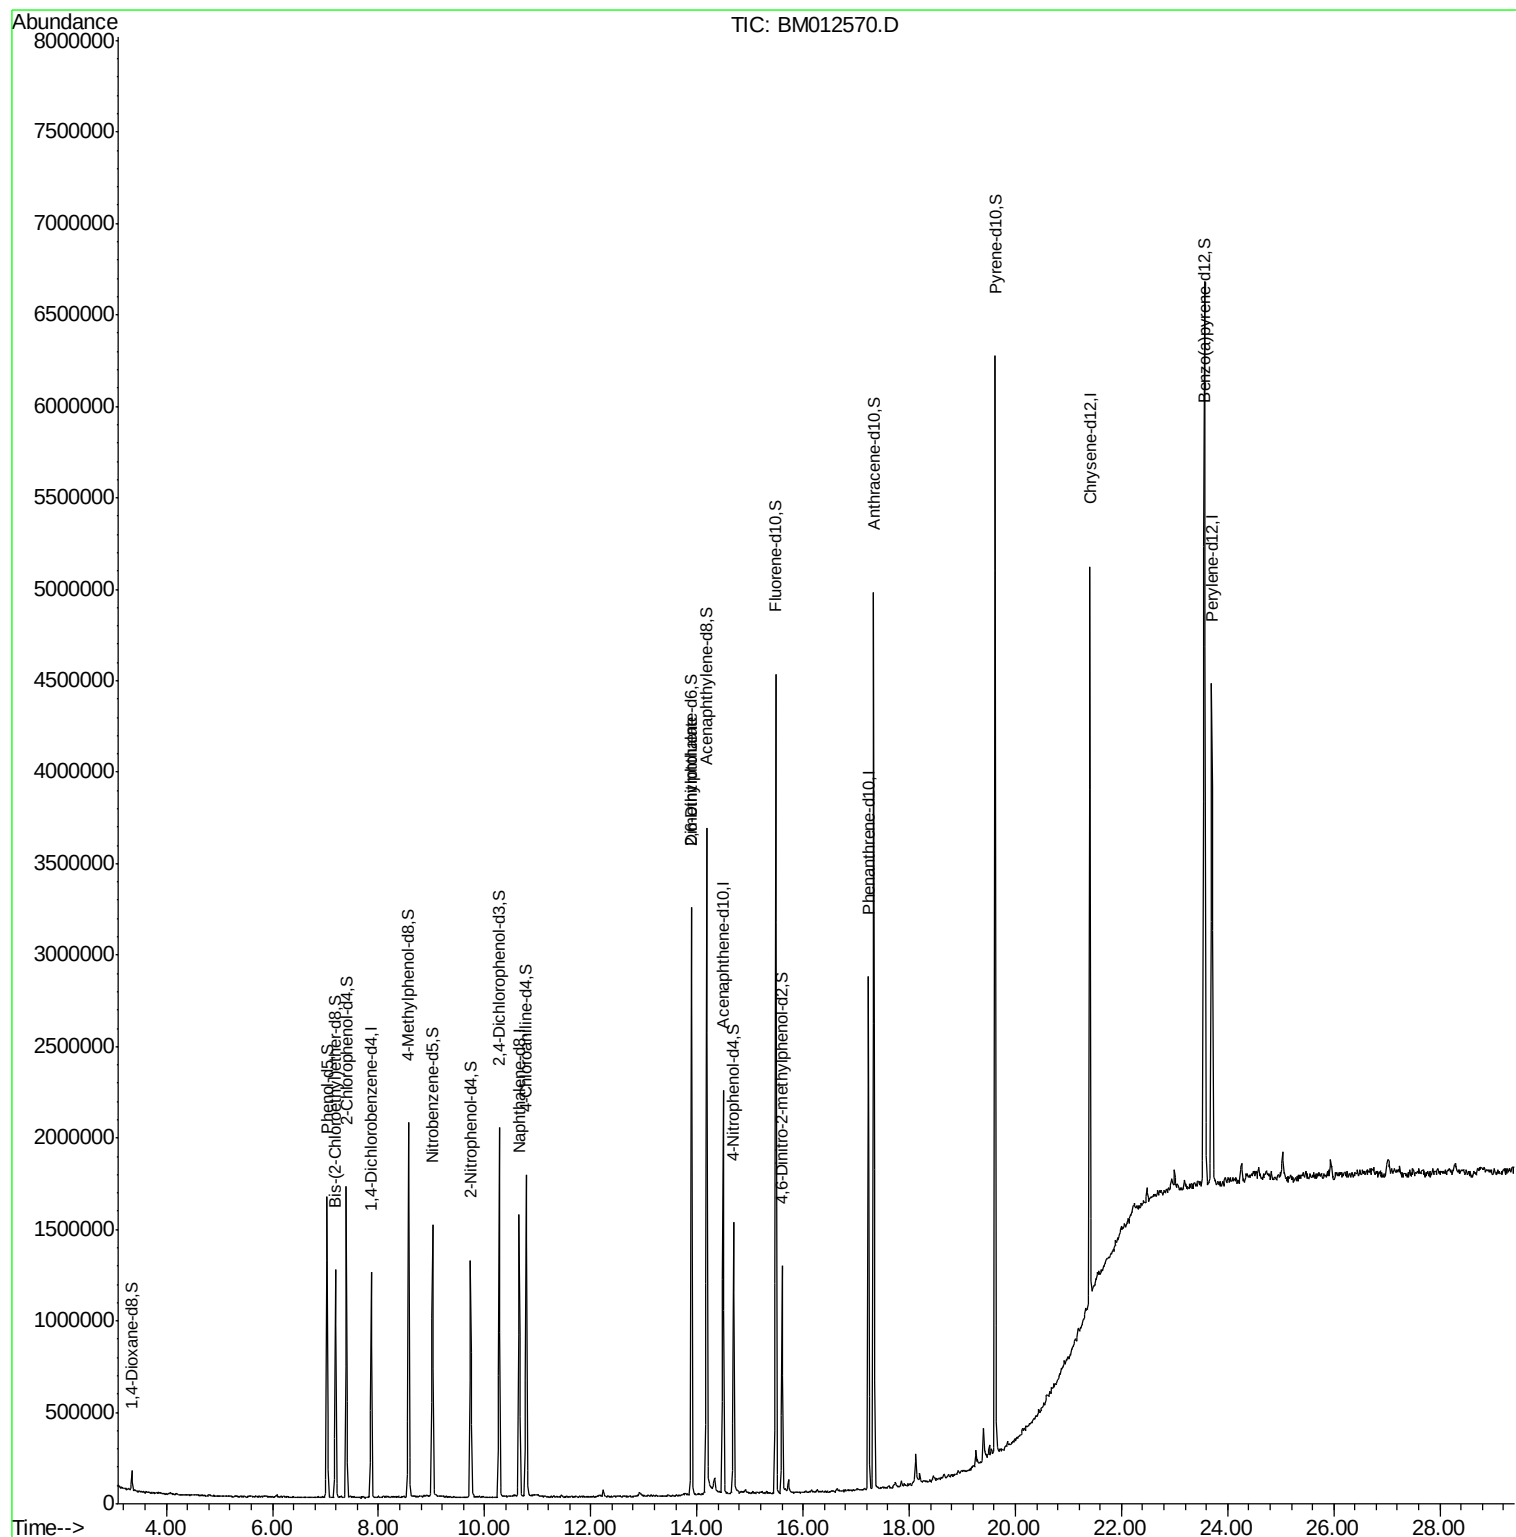

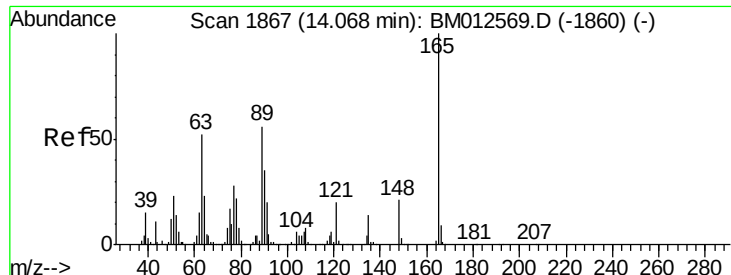

#45

2,6-Dinitrotoluene

Concen: 1.63 ng/ul

RT: 13.90 min Scan# 1839

Delta R.T. -0.16 min

Lab File: BM012570.D

Acq: 30 Oct 2017 13:16

Instrument :

BNA_M

ClientSampleId :



Tot Ion:165 Resp: 15616

Ion Ratio Lower Upper

165 100

89 0.0 52.6 79.0#

121 32.0 14.6 22.0#

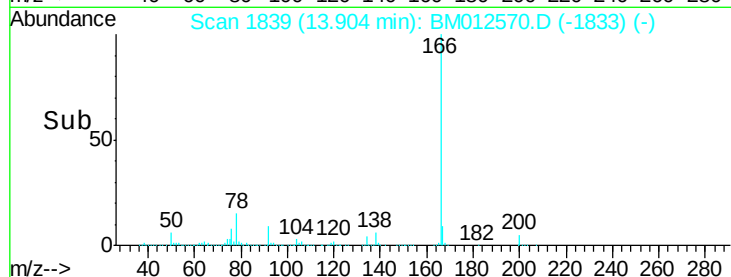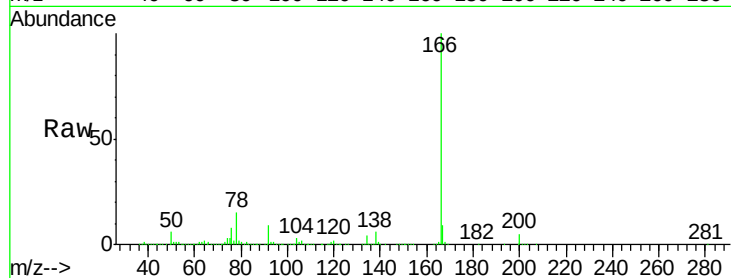

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

