

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
 Data File : BM012598.D
 Acq On : 31 Oct 2017 05:58
 Operator : SJ/JU
 Sample : I5786-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Oct 31 08:46:23 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 31 04:46:13 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
ClientSampleId :
 B-8(1.5-2.5) 101017

Manual Integrations
APPROVED

Sohil
 10/31/2017 7:47:41 PM

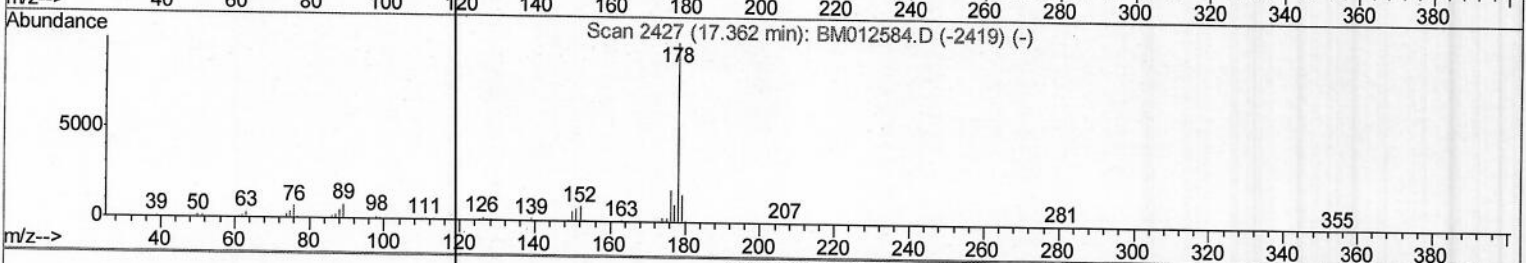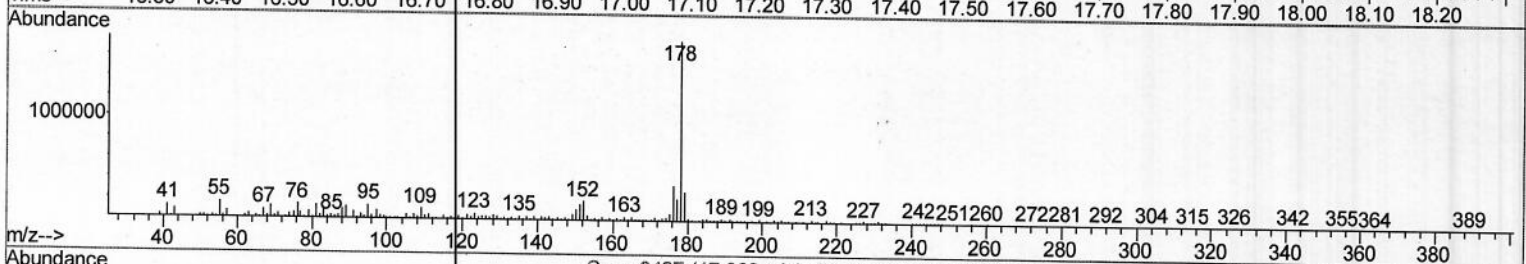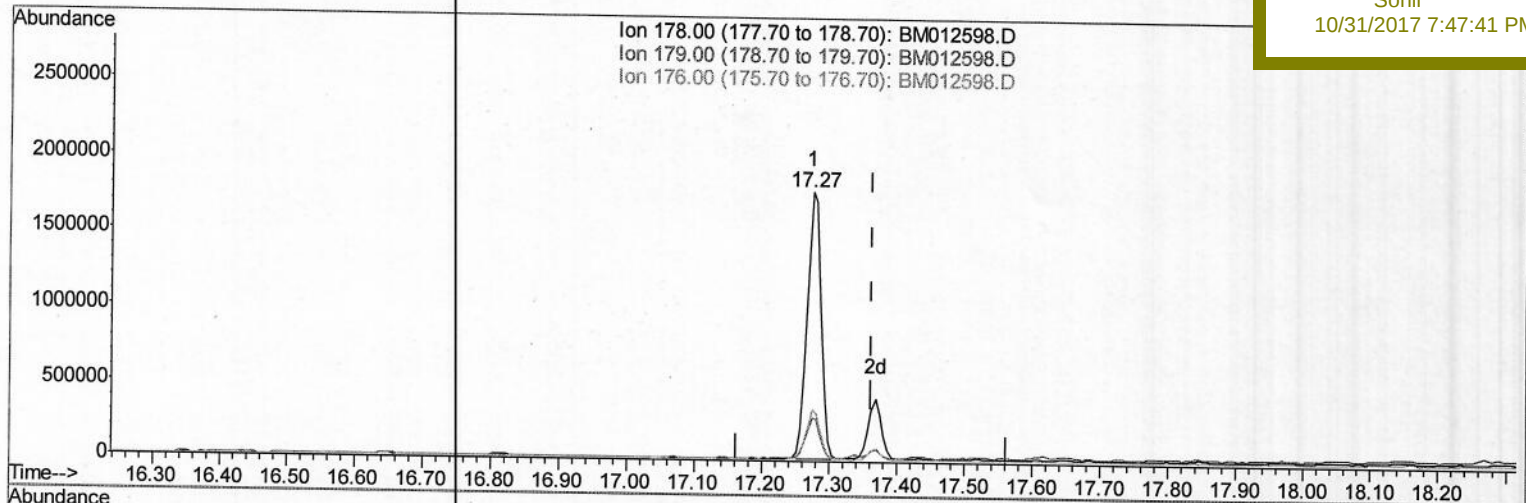

TIC: BM012598.D

(71) Anthracene

17.274min (-0.088) 25.83ng/ul

response 2537232

Ion	Exp%	Act%
178.00	100	100
179.00	14.60	16.48
176.00	18.20	19.69
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
Data File : BM012598.D
Acq On : 31 Oct 2017 05:58
Operator : SJ/JU
Sample : I5786-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Oct 31 08:46:23 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 31 04:46:13 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
B-8(1.5-2.5) 101017

Manual Integrations
APPROVED

Sohil
10/31/2017 7:47:41 PM

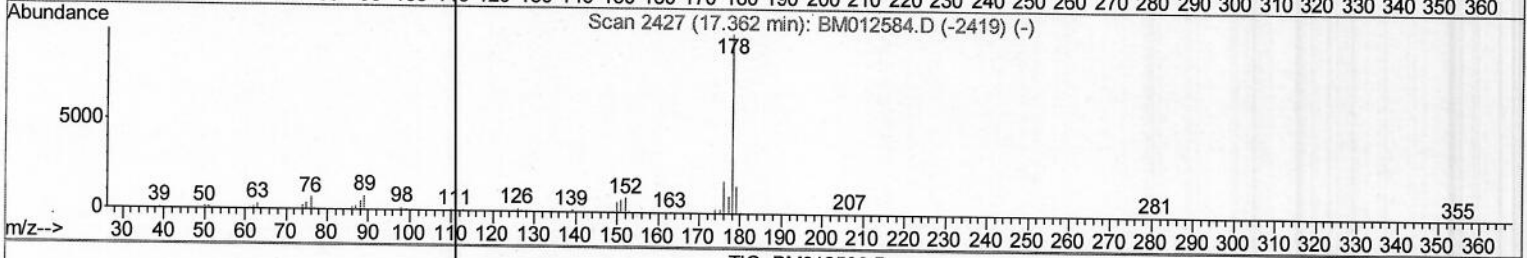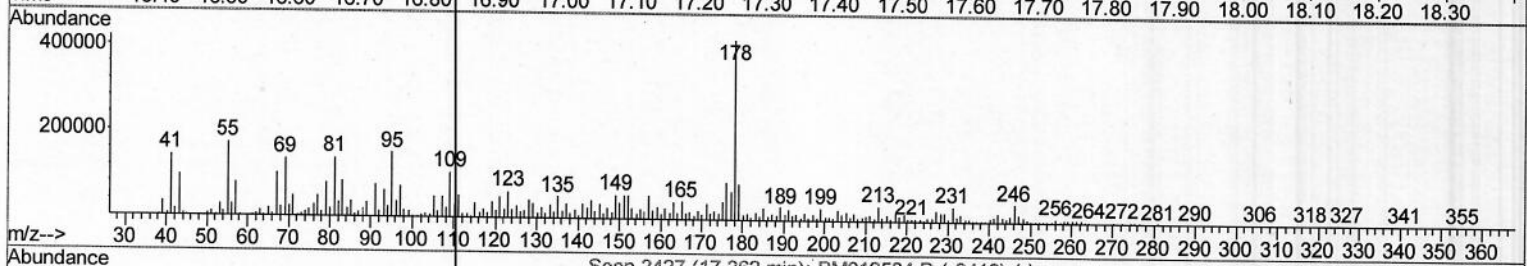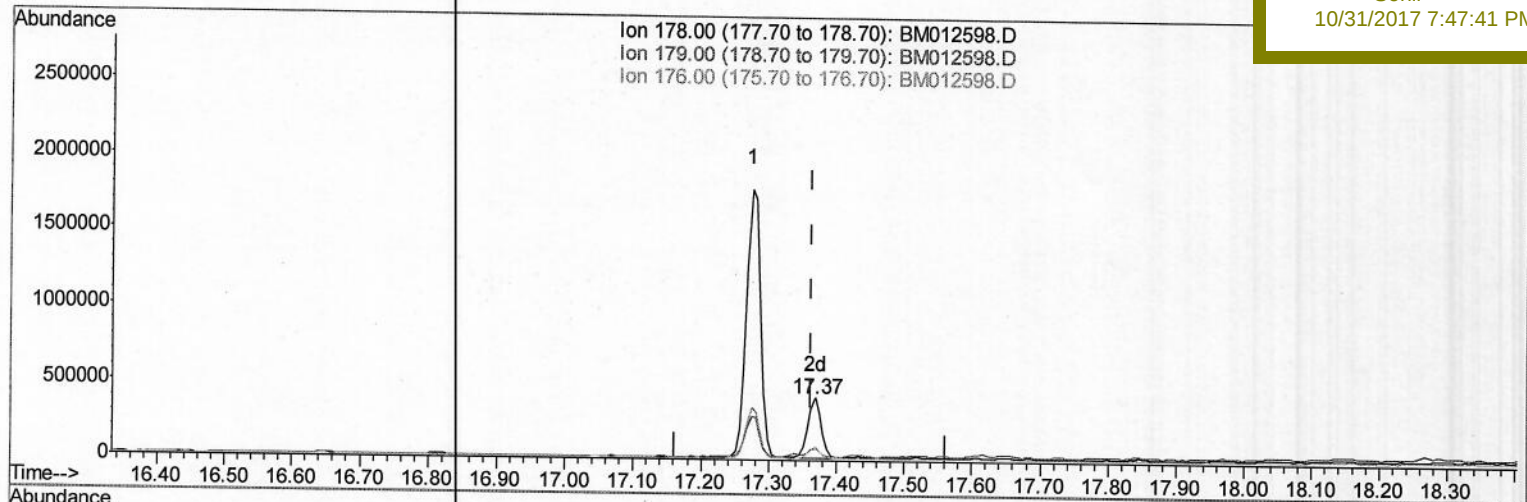

TIC: BM012598.D

(71) Anthracene

17.368min (+0.006) 5.51ng/ul m > SJ11/02117

response 541487

Ion	Exp%	Act%
178.00	100	100
179.00	14.60	19.81#
176.00	18.20	20.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
 Data File : BM012598.D
 Acq On : 31 Oct 2017 05:58
 Operator : SJ/JU
 Sample : I5786-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Oct 31 08:46:23 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 31 04:46:13 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 B-8(1.5-2.5) 101017

Manual Integrations
 APPROVED

Sohil
 10/31/2017 7:47:41 PM

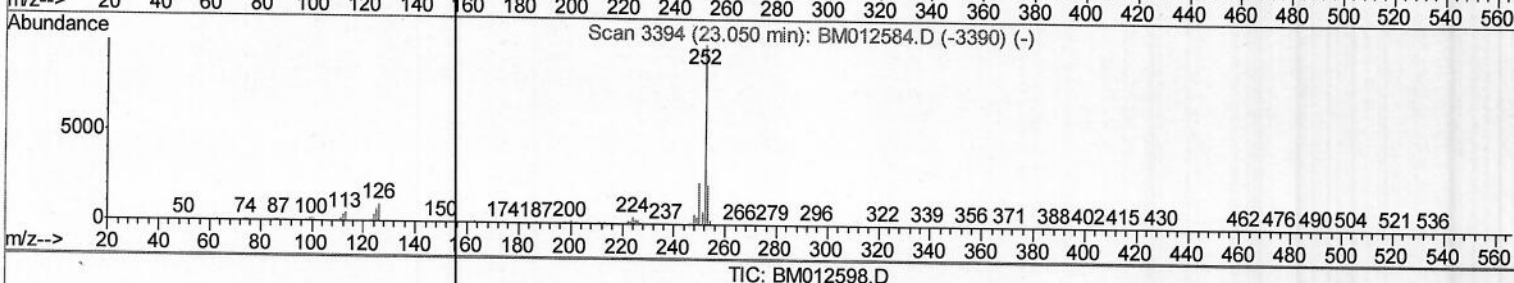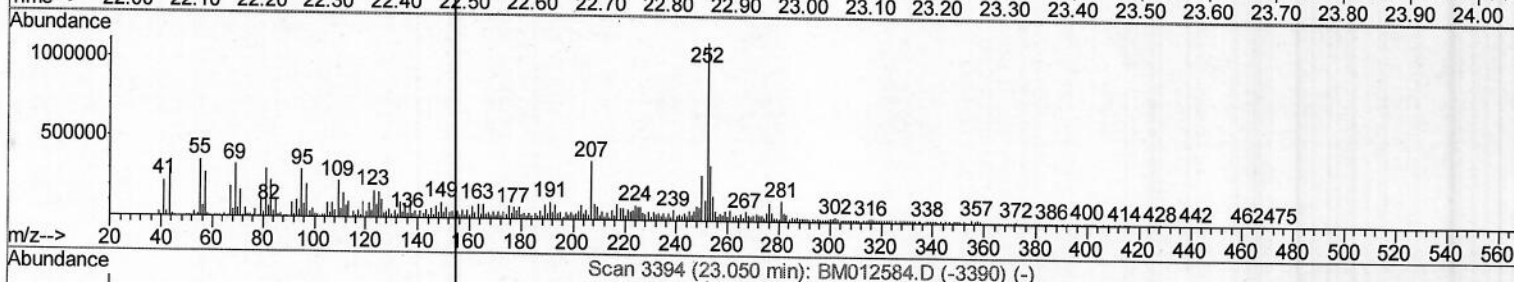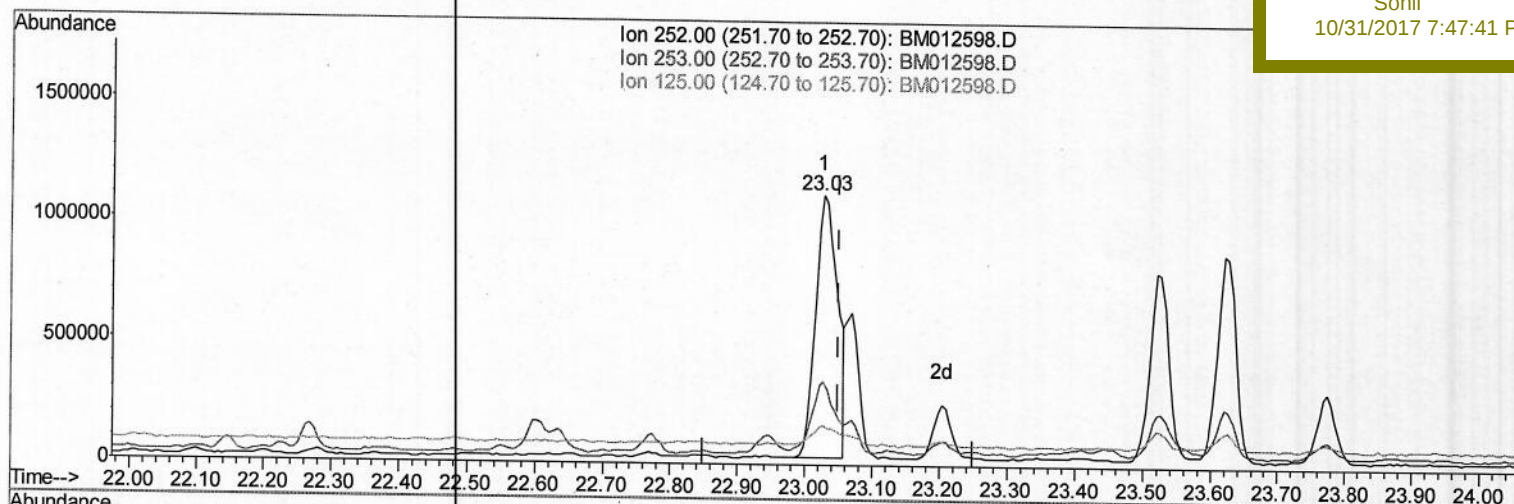

(86) Benzo(k)fluoranthene
 23.027min (-0.023) 17.34ng/ul
 response 2469043

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	30.70#
125.00	4.30	14.70#
0.00	0.00	0.00

TIC: BM012598.D

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
 Data File : BM012598.D
 Acq On : 31 Oct 2017 05:58
 Operator : SJ/JU
 Sample : I5786-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Oct 31 08:46:23 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 31 04:46:13 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 B-8(1.5-2.5) 101017

Manual Integrations
 APPROVED

Sohil
 10/31/2017 7:47:41 PM

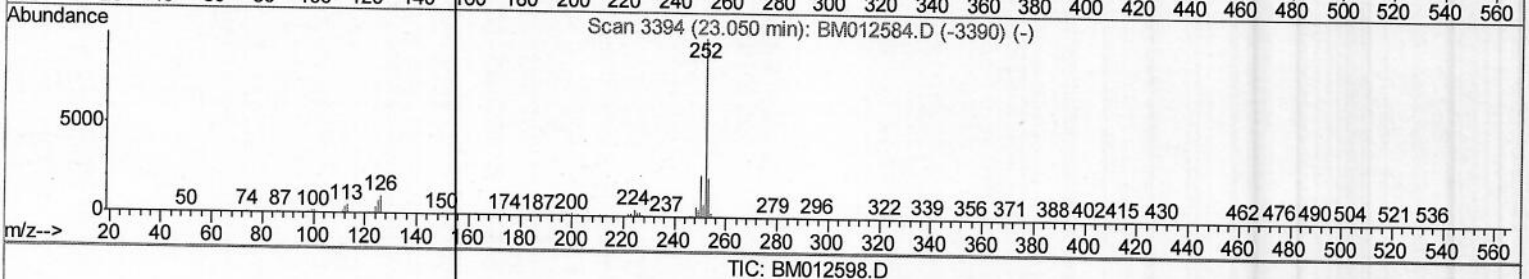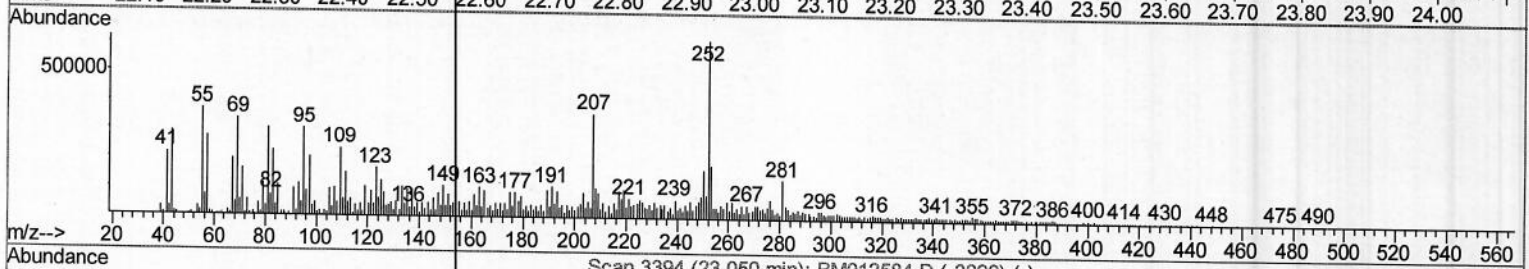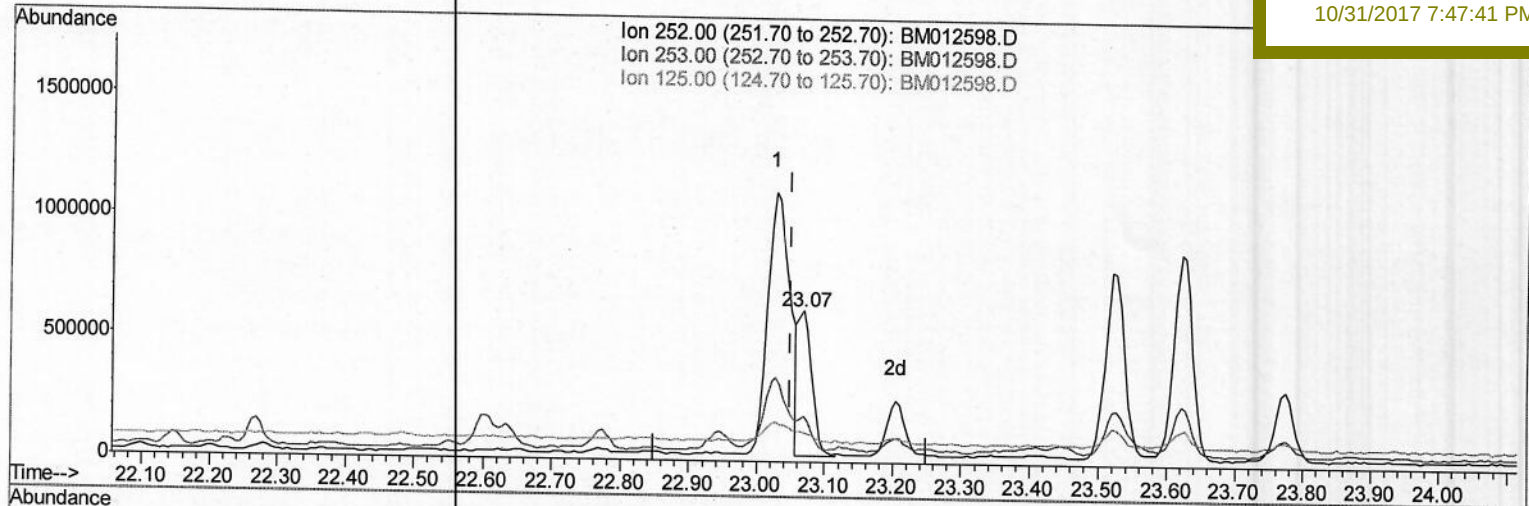

TIC: BM012598.D

(86) Benzo(k)fluoranthene

23.068min (+0.018) 5.70ng/ul m > 551102117

response 812215

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	29.81#
125.00	4.30	20.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
 Data File : BM012598.D
 Acq On : 31 Oct 2017 05:58
 Operator : SJ/JU
 Sample : I5786-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Oct 31 09:12:13 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 31 04:46:13 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 Client Sampled :
 B-8(1.5-2.5) 101017

Manual Integrations
 APPROVED

Sohil
 10/31/2017 7:47:41 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	343993	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	1329883	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	779910	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.23	188	1757158	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	2182067	20.00	ng/ul	0.00
83) Perylene-d12	23.72	264	2447927	20.00	ng/ul	0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.36	96	41488	6.16	ng/uL	0.00
5) Phenol-d5	7.03	99	858459	29.87	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.19	67	509360	29.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.39	132	692785	32.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.56	113	676688	27.55	ng/ul	0.00
19) Nitrobenzene-d5	9.02	128	336823	40.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	386942	45.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	740522	32.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.79	131	354836	14.81	ng/ul	0.00
43) Dimethylphthalate-d6	13.90	166	2131375	31.28	ng/ul	0.00
46) Acenaphthylene-d8	14.18	160	2701995	33.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	308693	30.48	ng/ul	0.00
57) Fluorene-d10	15.48	176	1882796	32.65	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	121232	14.26	ng/ul	0.00
70) Anthracene-d10	17.33	188	2973379	35.51	ng/ul	0.00
76) Pyrene-d10	19.63	212	3523208	35.19	ng/ul	0.01
87) Benzo(a)pyrene-d12	23.58	264	4073378	35.03	ng/ul	0.03

Target Compounds

					Ovalue
6) Phenol	7.06	94	131288	4.39 ng/ul#	82
44) Dimethylphthalate	13.95	163	1014183	15.05 ng/ul	99
47) Acenaphthylene	14.21	152	320503	4.17 ng/ul	96
69) Phenanthrene	17.27	178	2537232	26.70 ng/ul	98
71) Anthracene	17.37	178	541487m)	5.51 ng/ul	> SJ11/02117
72) Carbazole	17.63	167	250996	3.09 ng/ul#	80
74) Fluoranthene	19.29	202	3641299	33.82 ng/ul#	91
77) Pyrene	19.66	202	3405930	27.45 ng/ul#	91
80) Benzo(a)anthracene	21.40	228	1713165	13.11 ng/ul#	90
81) Bis(2-ethylhexyl)phthalate	21.32	149	306963	4.13 ng/ul#	90
82) Chrysene	21.44	228	1752212	15.08 ng/ul#	90
85) Benzo(b)fluoranthene	23.03	252	2469043	16.32 ng/ul#	80
86) Benzo(k)fluoranthene	23.07	252	812215m)	5.70 ng/ul	> SJ11/02117
88) Benzo(a)pyrene	23.62	252	1621540	11.24 ng/ul#	86
89) Indeno(1,2,3-cd)pyrene	26.07	276	1623932	9.56 ng/ul#	92
90) Dibenzo(a,h)anthracene	26.07	278	396185	2.75 ng/ul#	51
91) Benzo(g,h,i)perylene	26.80	276	1367464	9.94 ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
Data File : BM012598.D
Acq On : 31 Oct 2017 05:58
Operator : SJ/JU
Sample : I5786-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Oct 31 09:12:13 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 31 04:46:13 2017
Response via : Initial Calibration

Instrument :

BNA_M

Client Sampled :

B-8(1.5-2.5) 101017

Manual Integrations
APPROVED

Sohil

10/31/2017 7:47:41 PM

