

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
 Data File : BM012603.D
 Acq On : 31 Oct 2017 11:21
 Operator : SJ/JU
 Sample : I5873-03DL 30X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B-13(1-3)_101117DL

Quant Time: Oct 31 14:18:50 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 31 04:46:13 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	315004	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	1194642	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	682815	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.23	188	1561612	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	1856517	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	2148079	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.36	96	694	0.11	ng/uL	0.00
5) Phenol-d5	7.03	99	13358	0.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.19	67	8239	0.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.40	132	10489	0.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.57	113	8858	0.39	ng/ul	0.01
19) Nitrobenzene-d5	9.02	128	4738	0.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.74	143	4397	0.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.28	165	10294	0.50	ng/ul	0.01
29) 4-Chloroaniline-d4	10.79	131	1326	0.06	ng/ul	0.01
43) Dimethylphthalate-d6	13.90	166	31157	0.52	ng/ul	0.00
46) Acenaphthylene-d8	14.18	160	36825	0.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	3370	0.38	ng/ul	0.02
57) Fluorene-d10	15.48	176	28564	0.57	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.33	188	45133	0.61	ng/ul	0.00
76) Pyrene-d10	19.62	212	49706	0.58	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	55752	0.55	ng/ul	0.01

Target Compounds


				Ovalue
81) Bis(2-ethylhexyl)phthalate	21.32	149	4816276	76.106 ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
Data File : BM012603.D
Acq On : 31 Oct 2017 11:21
Operator : SJ/JU
Sample : I5873-03DL 30X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-13(1-3)_101117DL

Quant Time: Oct 31 14:18:50 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 31 04:46:13 2017
Response via : Initial Calibration

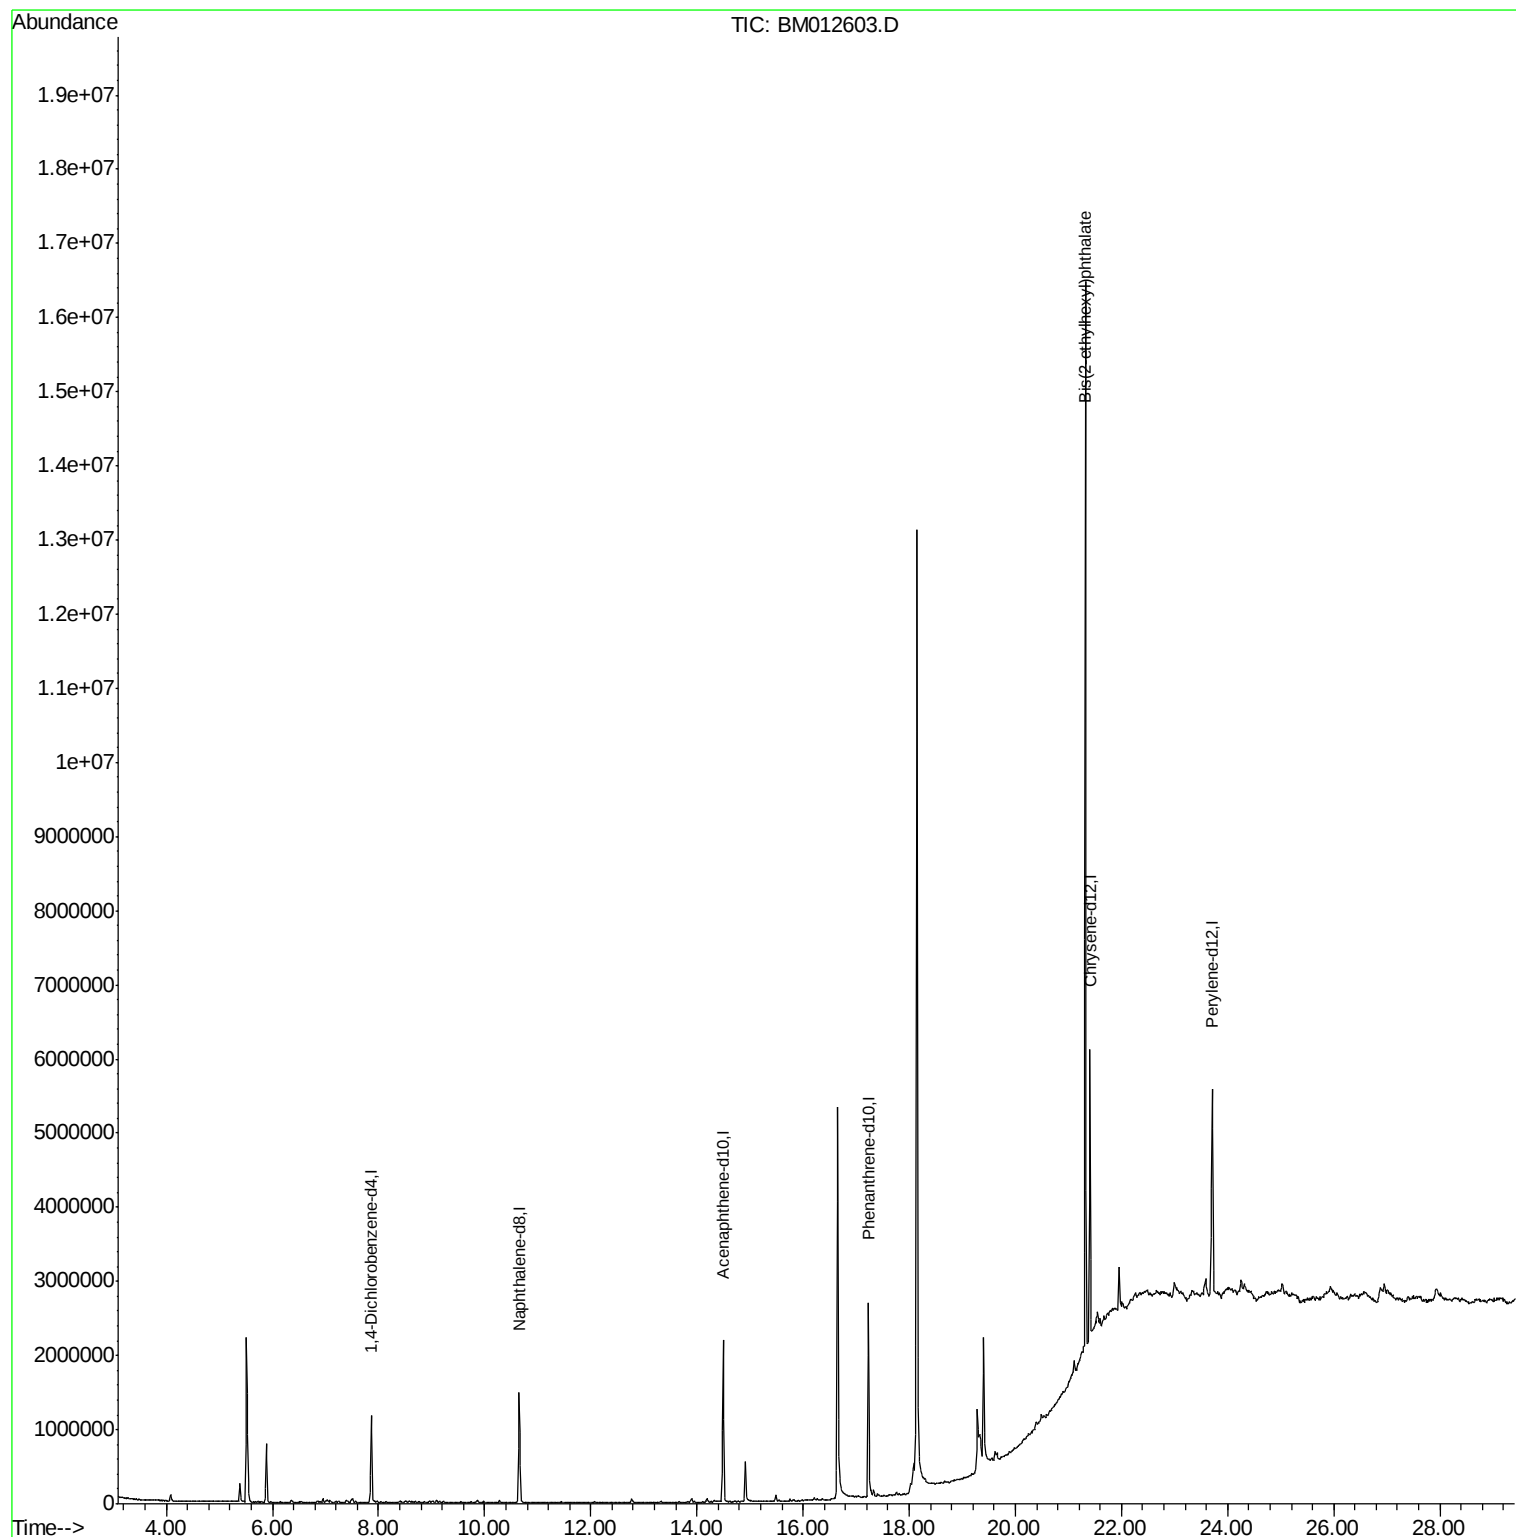

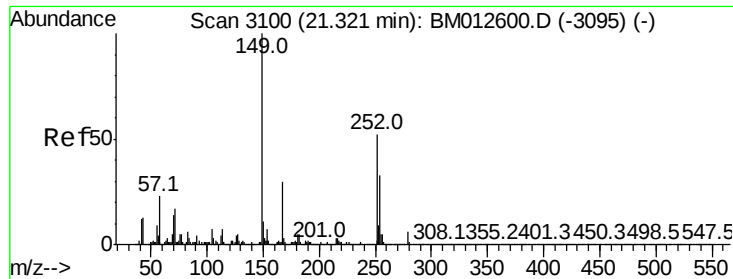

#81
 Bis(2-ethylhexyl)phthalate
 Concen: 76.106 ng/ul
 RT: 21.32 min Scan# 3100
 Delta R.T. 0.01 min
 Lab File: BM012603.D
 Acq: 31 Oct 2017 11:21

Instrument :
 BNA_M
 ClientSampleId :
 B-13(1-3)_101117DL

Tot Ion:149 Resp: 4816276
 Ion Ratio Lower Upper
 149 100
 167 29.2 22.8 34.2
 279 5.8 4.9 7.3

