




Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
Data File : BM012580.D
Acq On : 30 Oct 2017 19:15
Operator : SJ/JU
Sample : I5886-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNE1

Manual Integrations
APPROVED

Sohil
10/31/2017 7:47:09 PM

Quant Time: Oct 31 03:02:31 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 31 03:00:36 2017
Response via : Initial Calibration

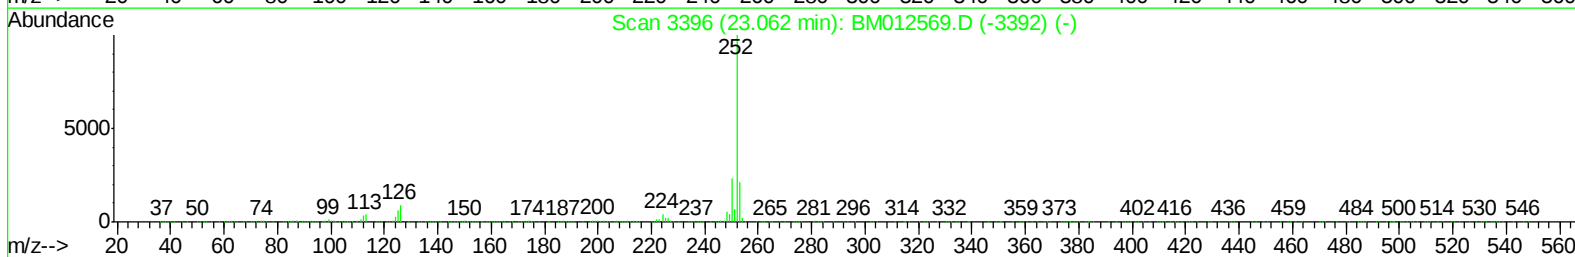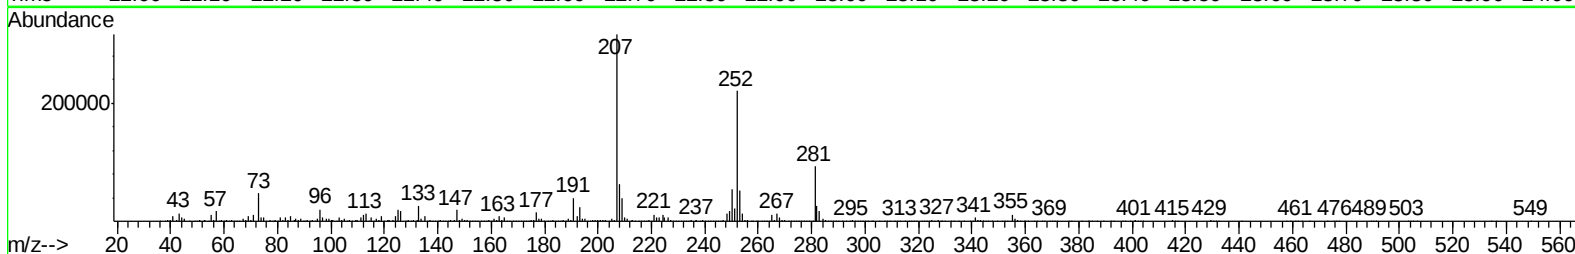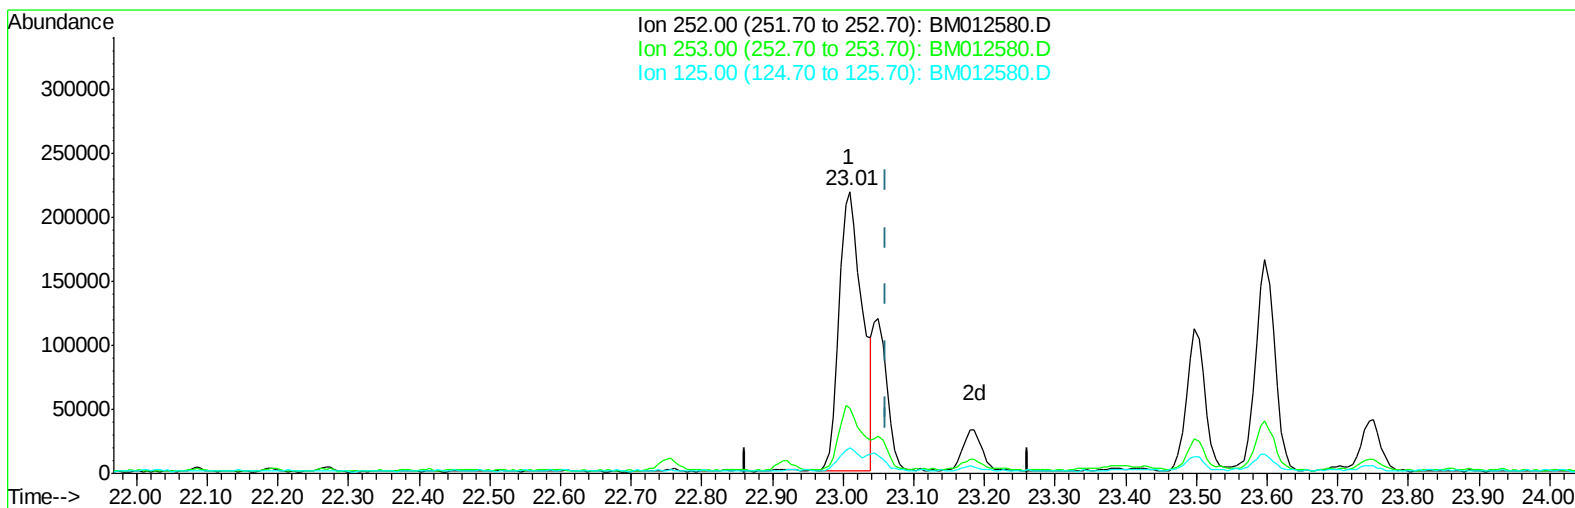

TIC: BM012580.D

(86) Benzo(k)fluoranthene

23.009min (-0.053) 4.57ng/ul

response 501955

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	23.42
125.00	4.30	9.26#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
Data File : BM012580.D
Acq On : 30 Oct 2017 19:15
Operator : SJ/JU
Sample : I5886-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNE1

Manual Integrations
APPROVED

Sohil
10/31/2017 7:47:09 PM

Quant Time: Oct 31 03:02:31 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 31 03:00:36 2017
Response via : Initial Calibration

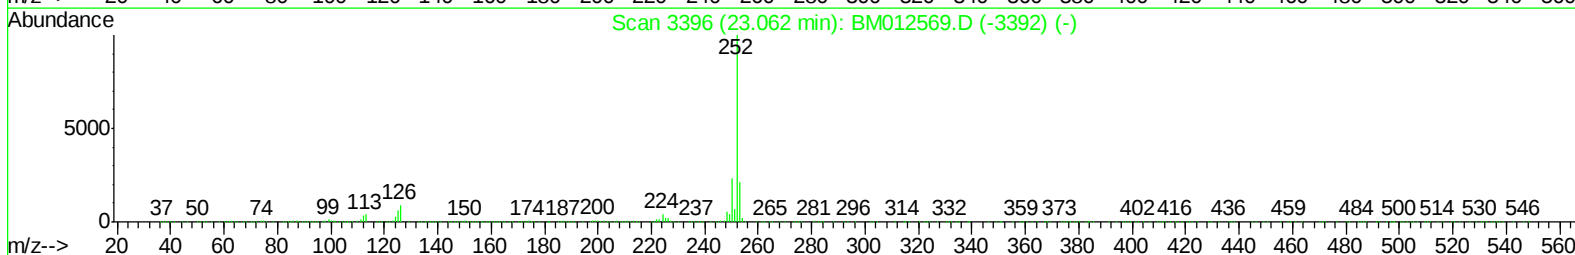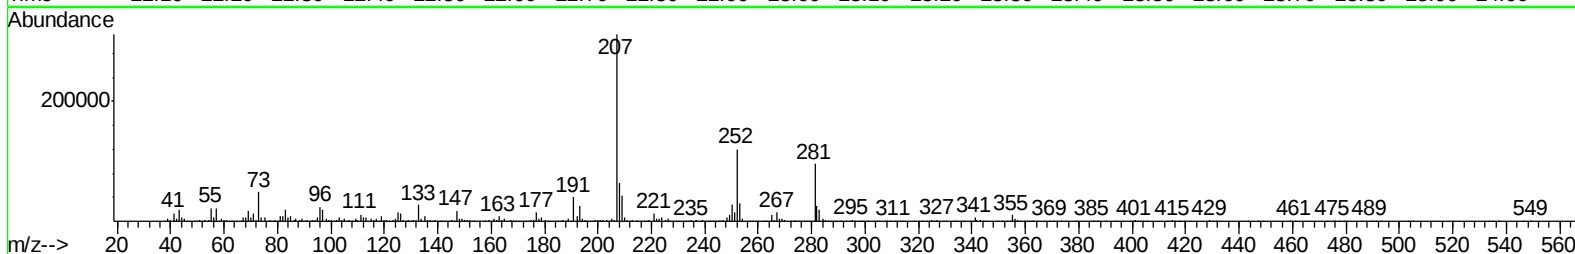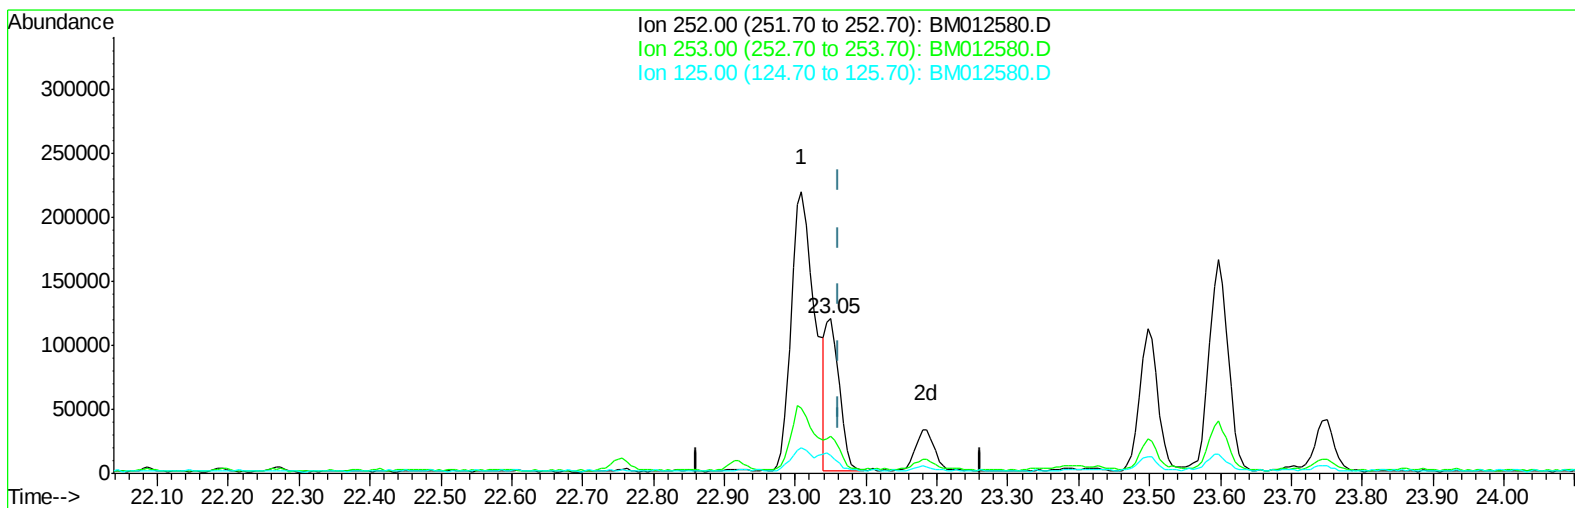

TIC: BM012580.D

(86) Benzo(k)fluoranthene

23.050min (-0.012) 1.48ng/ul m

response 162021

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	24.24
125.00	4.30	11.97#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
 Data File : BM012580.D
 Acq On : 30 Oct 2017 19:15
 Operator : SJ/JU
 Sample : I5886-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESNE1

Manual Integrations
 APPROVED

Sohil
 10/31/2017 7:47:09 PM

Quant Time: Oct 31 04:23:19 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 31 03:00:36 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	300390	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	1134681	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	638560	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.23	188	1438648	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1696651	20.00	ng/ul	0.00
83) Perylene-d12	23.70	264	1887265	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.35	96	29231	4.97	ng/uL	0.00
5) Phenol-d5	7.02	99	503239	20.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.19	67	331679	22.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.39	132	427124	22.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.56	113	326070	15.20	ng/ul	0.00
19) Nitrobenzene-d5	9.01	128	203056	28.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	227171	31.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	416950	21.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.78	131	432899	21.17	ng/ul	0.00
43) Dimethylphthalate-d6	13.90	166	1261276	22.61	ng/ul	0.00
46) Acenaphthylene-d8	14.18	160	1544283	23.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	154064	18.58	ng/ul	0.00
57) Fluorene-d10	15.48	176	1072030	22.70	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.60	200	151764	21.80	ng/ul	0.00
70) Anthracene-d10	17.33	188	1568726	22.88	ng/ul	0.00
76) Pyrene-d10	19.62	212	1817035	23.34	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.55	264	2010468	22.42	ng/ul	-0.01

Target Compounds

						Ovalue
6) Phenol	7.05	94	79639	3.05	ng/ul#	86
44) Dimethylphthalate	13.94	163	76036	1.38	ng/ul	99
69) Phenanthrene	17.27	178	187559	2.41	ng/ul	99
74) Fluoranthene	19.29	202	704884	8.00	ng/ul#	93
77) Pyrene	19.64	202	587312	6.09	ng/ul#	91
80) Benzo(a)anthracene	21.39	228	432684	4.26	ng/ul	97
81) Bis(2-ethylhexyl)phthalate	21.31	149	66748	1.15	ng/ul	99
82) Chrysene	21.44	228	403388	4.47	ng/ul	99
85) Benzo(b)fluoranthene	23.01	252	501955	4.30	ng/ul#	96
86) Benzo(k)fluoranthene	23.05	252	162021m	1.48	ng/ul	
88) Benzo(a)pyrene	23.60	252	312567	2.81	ng/ul#	95
89) Indeno(1,2,3-cd)pyrene	26.03	276	211400	1.61	ng/ul#	96
91) Benzo(g,h,i)perylene	26.74	276	149011	1.40	ng/ul#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103017\
Data File : BM012580.D
Acq On : 30 Oct 2017 19:15
Operator : SJ/JU
Sample : I5886-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNE1

Quant Time: Oct 31 04:23:19 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 31 03:00:36 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
10/31/2017 7:47:09 PM

