

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM103017\
 Data File : BM012575.D
 Acq On : 30 Oct 2017 16:15
 Operator : SJ/JU
 Sample : I6127-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDEC2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102417.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	41	45	51	rVB	98282	126291	1.33%	0.156%
2	7.028	663	670	679	rVB	412936	656608	6.93%	0.811%
3	7.187	690	697	707	rBV	1175932	1810978	19.11%	2.238%
4	7.393	724	732	740	rBV	1429267	2200200	23.22%	2.719%
5	7.858	804	811	819	rVB	1314464	2134738	22.53%	2.638%
6	8.563	923	931	939	rBV	1082725	1726056	18.22%	2.133%
7	9.010	1000	1007	1018	rVB	1467647	2428012	25.63%	3.001%
8	9.734	1119	1130	1139	rBV	1264742	2079263	21.95%	2.570%
9	10.269	1212	1221	1232	rBV	1794618	3039573	32.08%	3.757%
10	10.646	1277	1285	1294	rBV	1646813	2789302	29.44%	3.447%
11	13.898	1831	1838	1849	rBV	3297223	4346059	45.87%	5.371%
12	14.181	1877	1886	1900	rBV	3649824	5313145	56.08%	6.566%
13	14.322	1905	1910	1924	rVB2	84613	206326	2.18%	0.255%
14	14.486	1931	1938	1947	rVB2	2207353	3488666	36.82%	4.312%
15	14.686	1965	1972	1981	rBV	352978	557517	5.88%	0.689%
16	15.481	2100	2107	2115	rBV	4662205	6493596	68.54%	8.025%
17	15.604	2122	2128	2141	rBV	1384144	1934552	20.42%	2.391%
18	15.722	2143	2148	2156	rVB	62721	103245	1.09%	0.128%
19	17.233	2398	2405	2411	rBV2	2896678	4093010	43.20%	5.058%
20	17.327	2415	2421	2430	rVV	5099720	7203699	76.03%	8.903%
21	18.122	2552	2556	2562	rBV4	93156	136844	1.44%	0.169%
22	19.398	2770	2773	2779	rBV2	117206	162939	1.72%	0.201%
23	19.616	2805	2810	2817	rBV	6085642	8199094	86.54%	10.133%
24	21.404	3109	3114	3120	rBV	3971671	4939486	52.13%	6.105%
25	23.557	3474	3480	3490	rVB2	4900127	9474576	100.00%	11.709%
26	23.704	3499	3505	3515	rVB2	2670211	5270634	55.63%	6.514%


Sum of corrected areas: 80914409

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM103017\
Data File : BM012575.D
Acq On : 30 Oct 2017 16:15
Operator : SJ/JU
Sample : I6127-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDEC2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

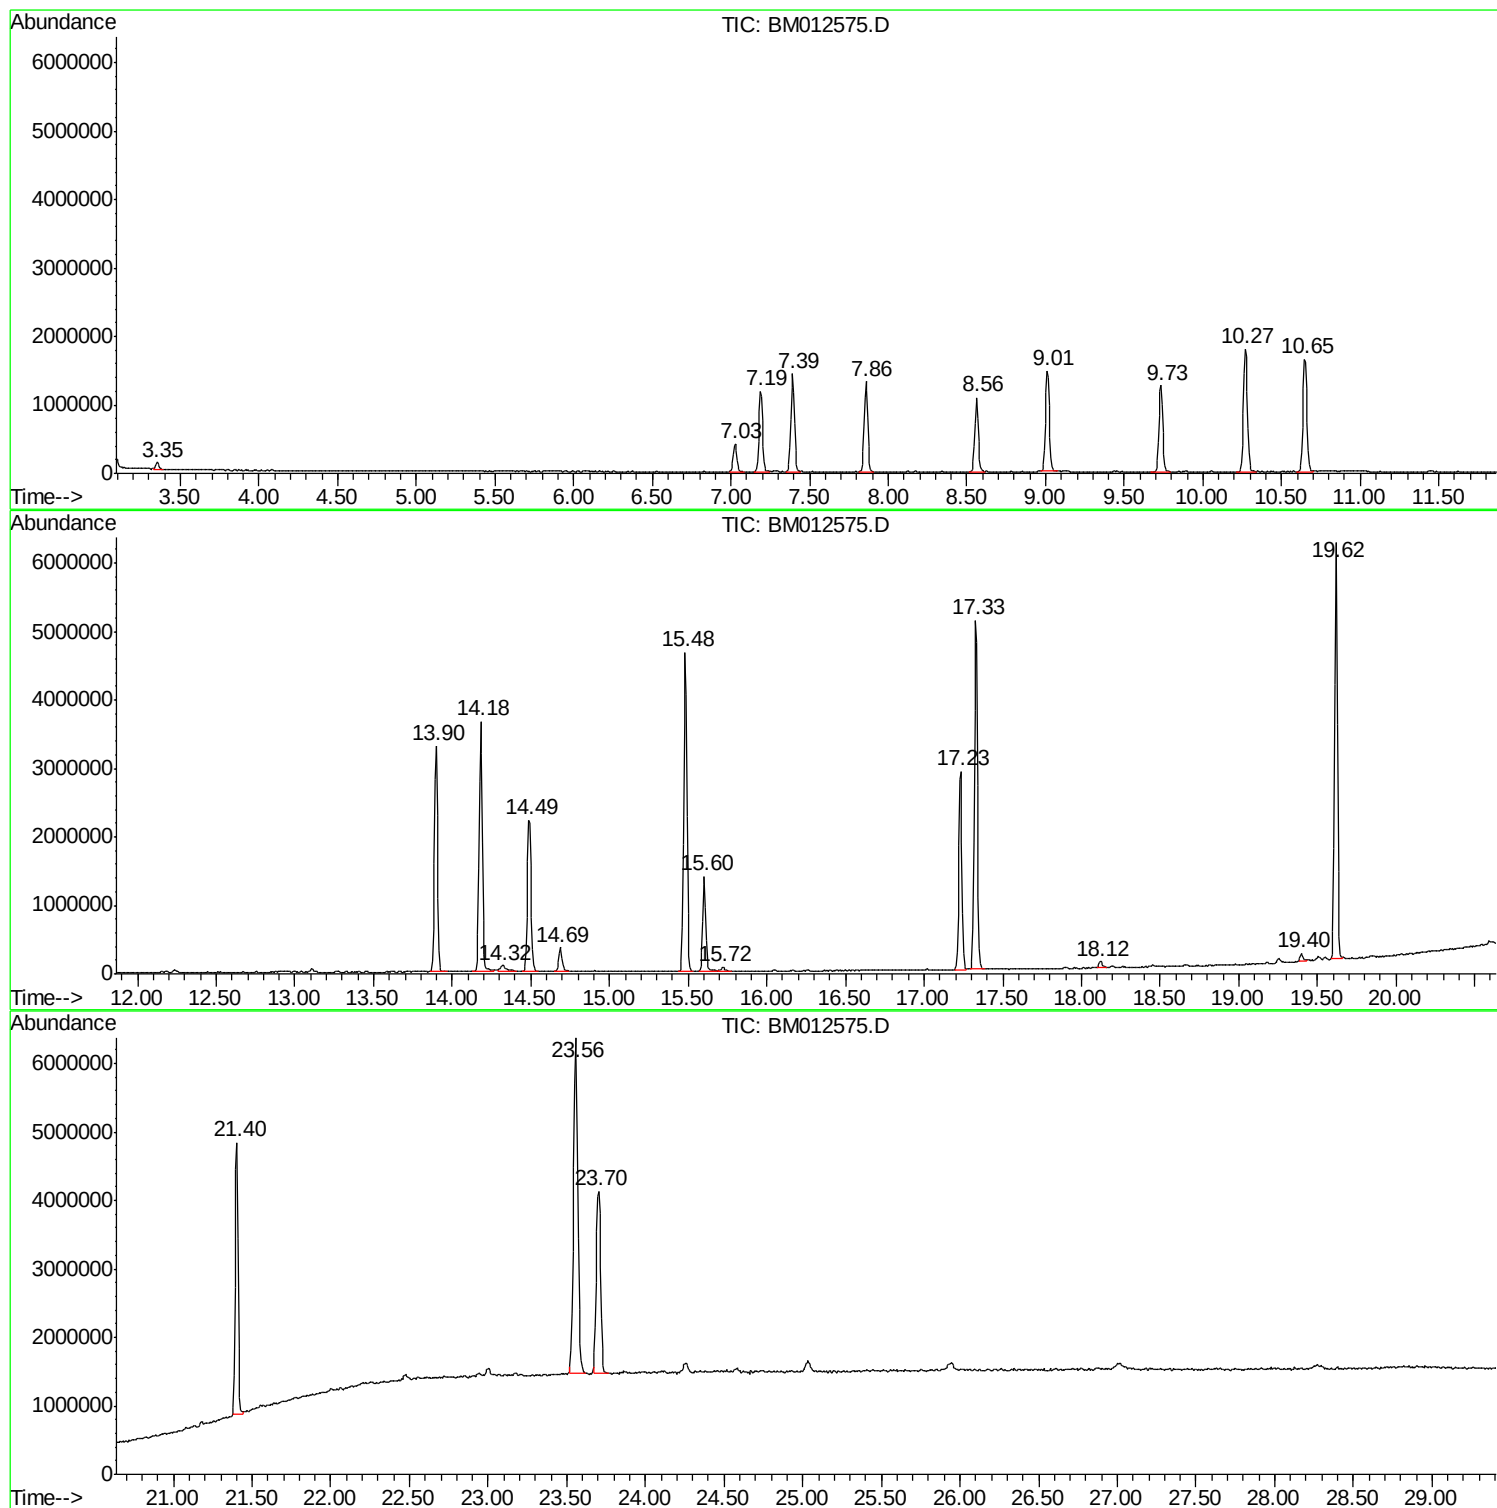

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM103017\
Data File : BM012575.D
Acq On : 30 Oct 2017 16:15
Operator : SJ/JU
Sample : I6127-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDEC2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM103017\
Data File : BM012575.D
Acq On : 30 Oct 2017 16:15
Operator : SJ/JU
Sample : I6127-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDEC2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc