


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103020\
 Data File : BM027657.D
 Acq On : 30 Oct 2020 12:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 30 17:56:42 2020

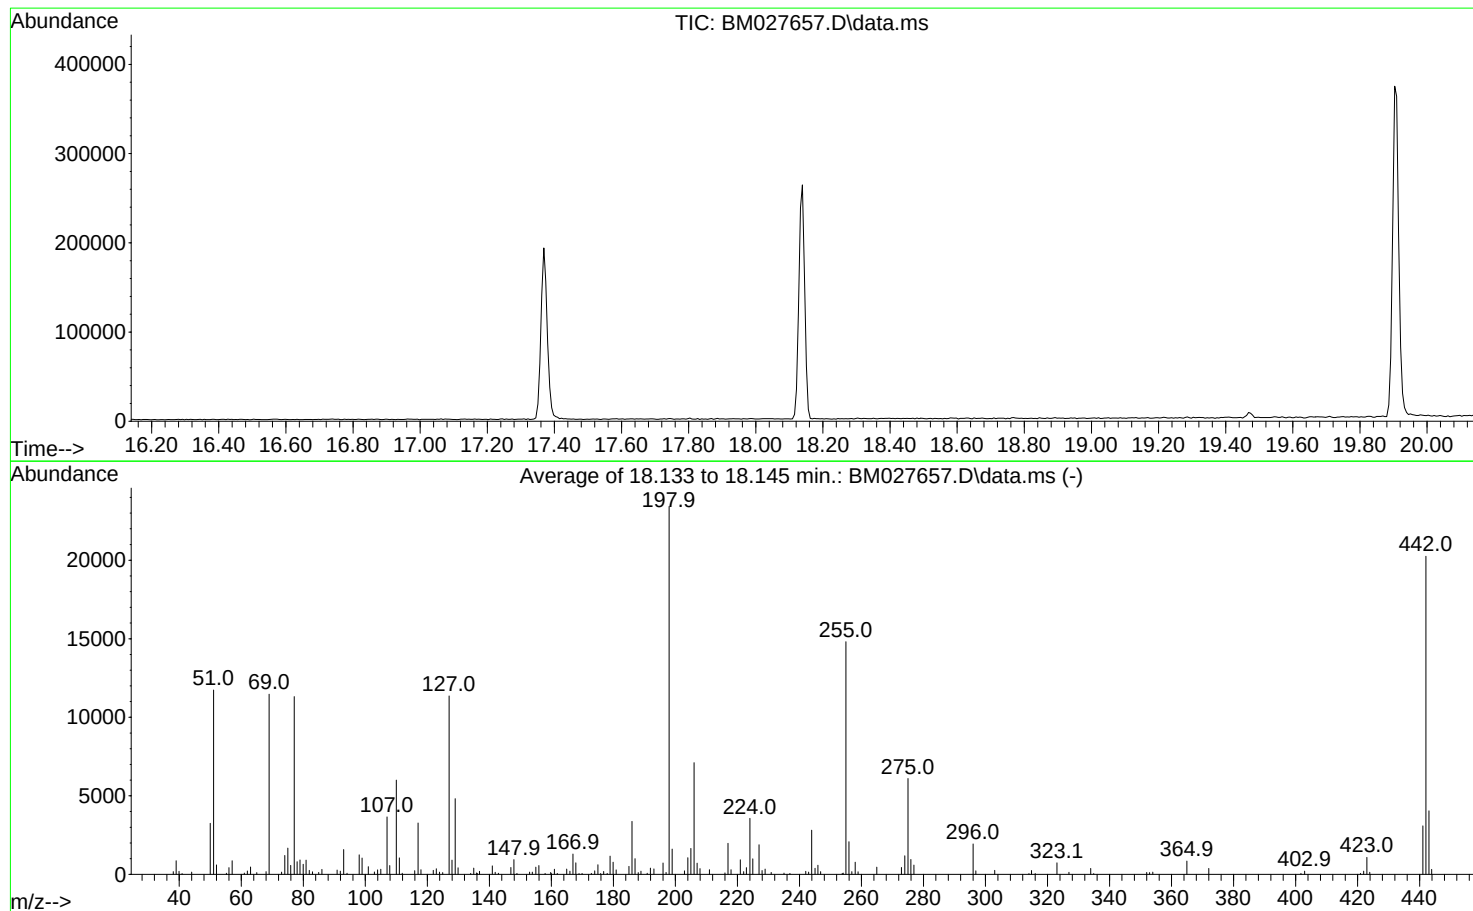

Spectrum Information: Average of 18.133 to 18.145 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	11741	PASS
68	69	0.00	2	1.5	172	PASS
69	198	0.00	100	49.0	11474	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	11358	PASS
197	198	0.00	2	0.5	125	PASS
198	198	100	100	100.0	23421	PASS
199	198	5	9	6.9	1611	PASS
275	198	10	60	26.0	6101	PASS
365	198	1	100	3.6	846	PASS
441	198	0.01	100	13.2	3092	PASS
442	198	50	100	86.5	20256	PASS
443	442	15	24	20.0	4047	PASS