

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103117\
 Data File : BM012614.D
 Acq On : 31 Oct 2017 21:47
 Operator : SJ/JU
 Sample : I5844-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 01 05:27:48 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 01 05:26:13 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	419194	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	1840348	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.49	164	1240827	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.23	188	2686943	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	2027507	20.00	ng/ul	0.00
83) Perylene-d12	23.69	264	2098455	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.35	96	44887	5.47	ng/uL	0.00
5) Phenol-d5	7.02	99	986297	28.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.18	67	596799	28.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.39	132	759812	28.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.56	113	879720	29.39	ng/ul	0.00
19) Nitrobenzene-d5	9.01	128	405415	35.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	477518	40.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.26	165	916572	29.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	1124461	33.90	ng/ul	0.00
43) Dimethylphthalate-d6	13.89	166	3215262	29.66	ng/ul	0.00
46) Acenaphthylene-d8	14.17	160	3841398	29.96	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	400648	24.86	ng/ul	0.00
57) Fluorene-d10	15.47	176	2662704	29.02	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.60	200	302828	23.29	ng/ul	0.00
70) Anthracene-d10	17.33	188	3943811	30.80	ng/ul	0.00
76) Pyrene-d10	19.62	212	3668312	39.44	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.55	264	3107335	31.17	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	7.05	94	78716	2.16	ng/ul#	81
44) Dimethylphthalate	13.94	163	1026828	9.58	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103117\
Data File : BM012614.D
Acq On : 31 Oct 2017 21:47
Operator : SJ/JU
Sample : I5844-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 01 05:27:48 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 01 05:26:13 2017
Response via : Initial Calibration

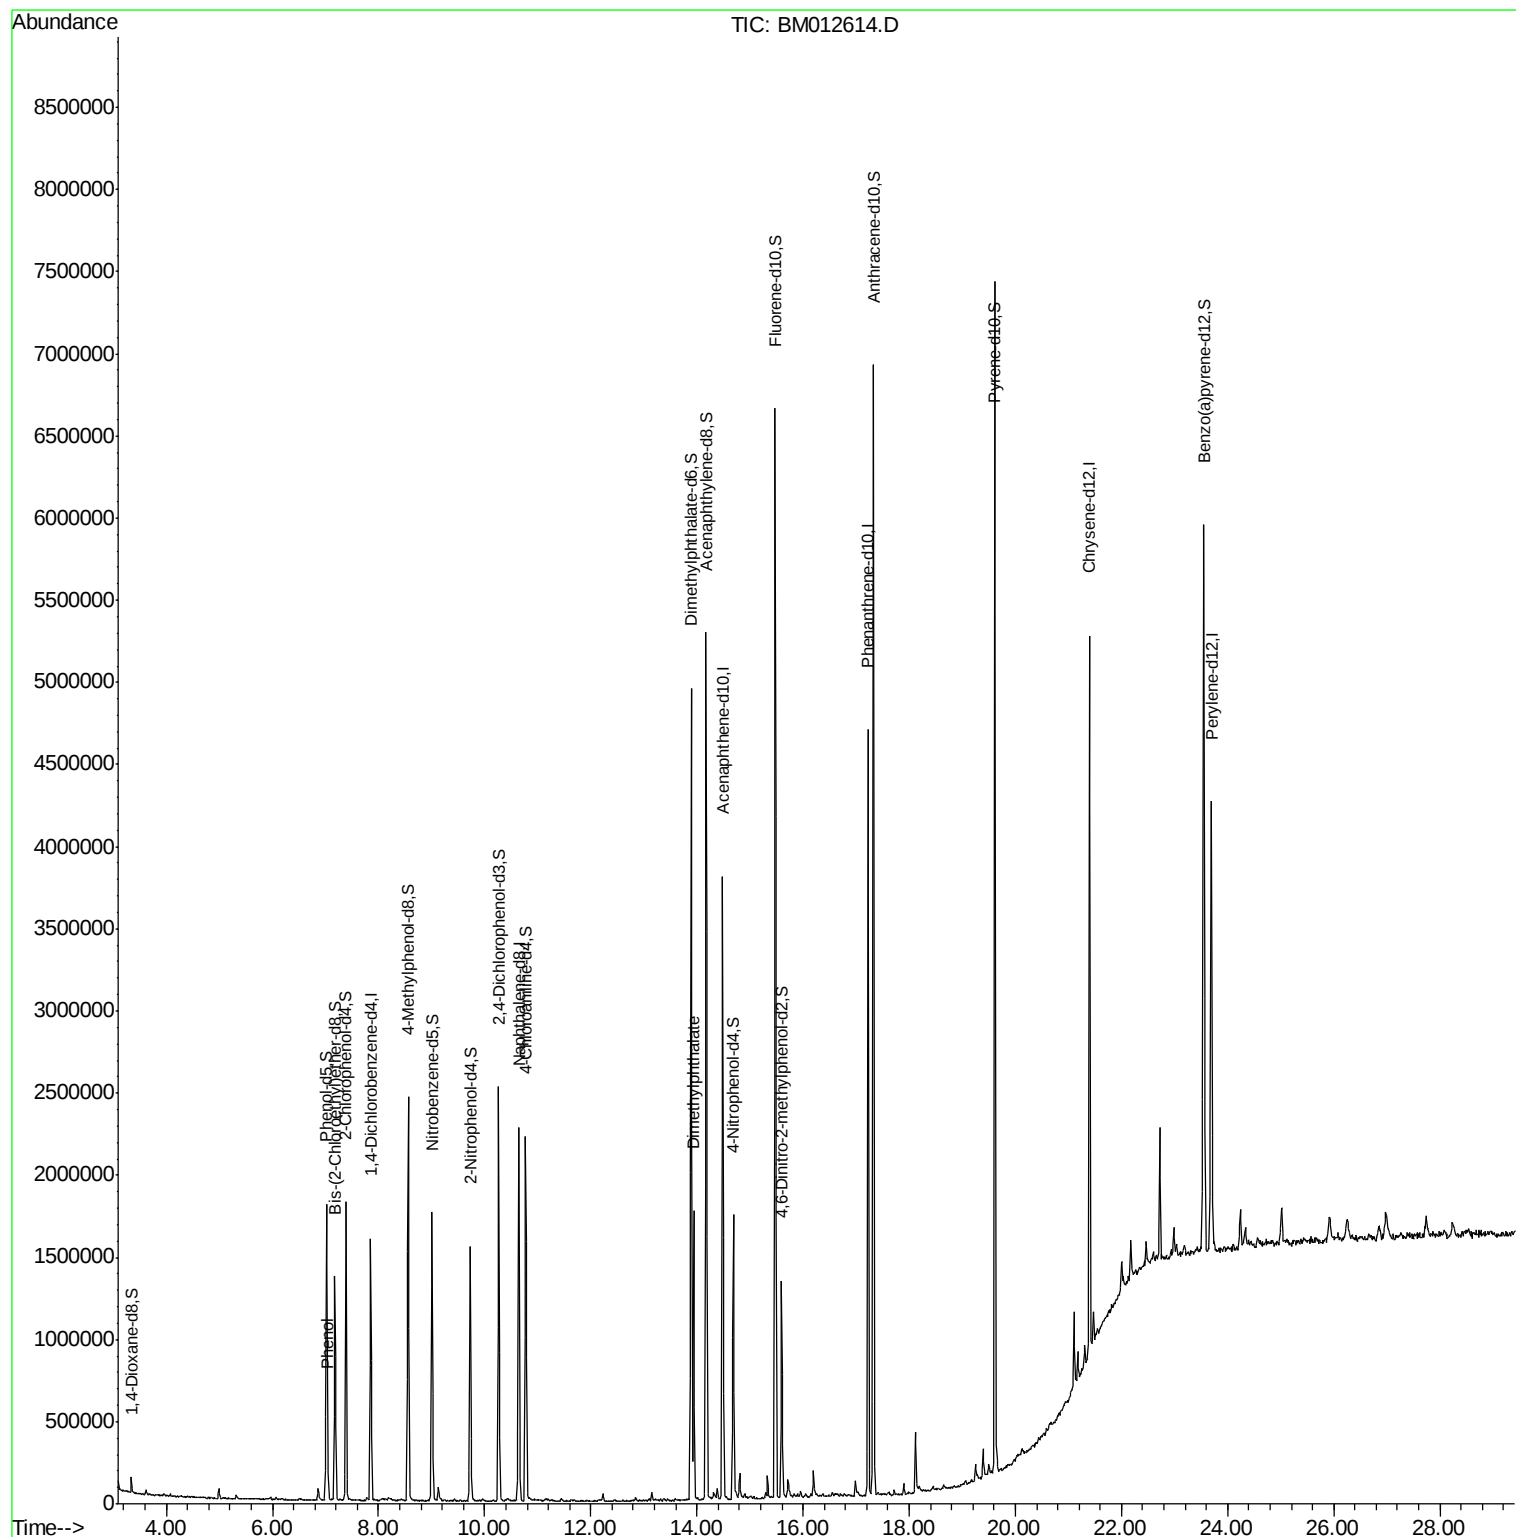

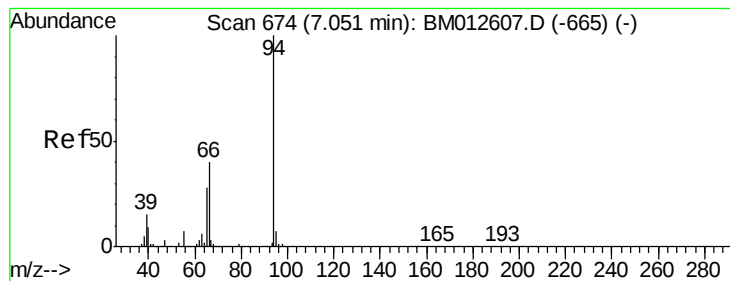

#6

Phenol

Concen: 2.16 ng/ul

RT: 7.05 min Scan# 673

Delta R.T. -0.01 min

Lab File: BM012614.D

Acq: 31 Oct 2017 21:47

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 94 Resp: 78716

Ion Ratio Lower Upper

94 100

65 28.6 28.2 42.4




66 41.4 47.2 70.8#

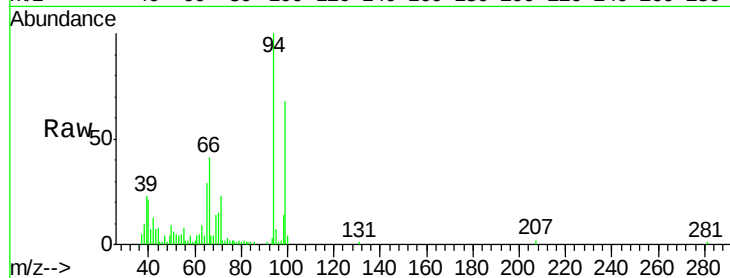

Abundance Ion 94.00 (93.70 to 94.70): BM012607.D (-665) (-)

Ion 65.00 (64.70 to 65.70): BM012607.D (-665) (-)

Ion 66.00 (65.70 to 66.70): BM012607.D (-665) (-)

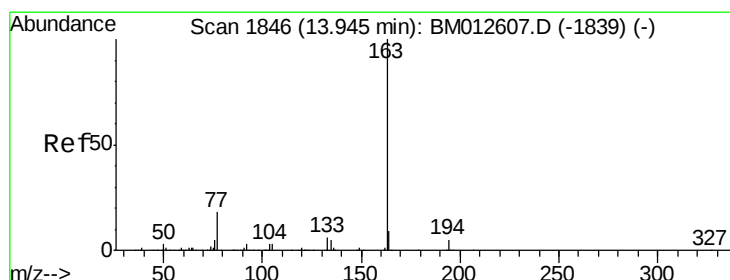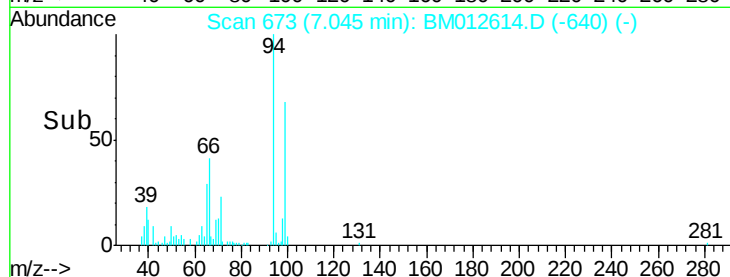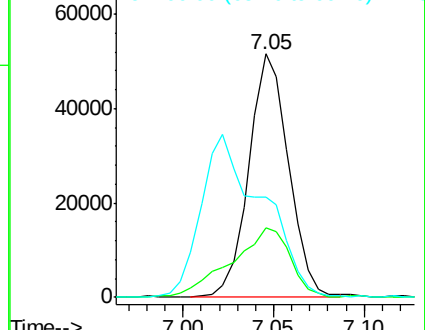

#44

Dimethylphthalate

Concen: 9.58 ng/ul

RT: 13.94 min Scan# 1845

Delta R.T. -0.01 min

Lab File: BM012614.D

Acq: 31 Oct 2017 21:47


Tgt Ion:163 Resp: 1026828

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 10.3 8.2 12.4

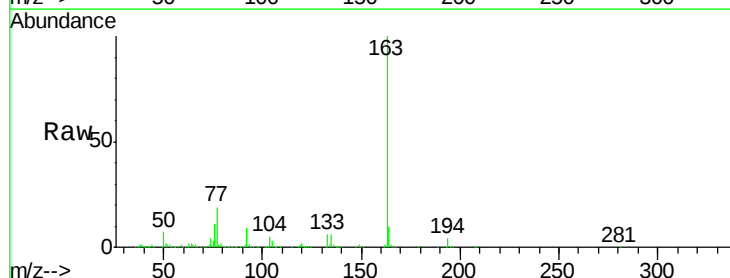

Abundance Ion 163.00 (162.70 to 163.70): BM012607.D (-1839) (-)

Ion 194.00 (193.70 to 194.70): BM012607.D (-1839) (-)

Ion 164.00 (163.70 to 164.70): BM012607.D (-1839) (-)

