

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103117\
 Data File : BM012620.D
 Acq On : 01 Nov 2017 01:20
 Operator : SJ/JU
 Sample : I6150-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 01 05:29:16 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 01 05:26:13 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	371569	20.00	ng/ul	0.00
18) Naphthalene-d8	10.64	136	1595843	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.48	164	1073499	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	2505169	20.00	ng/ul	-0.01
75) Chrysene-d12	21.40	240	2522638	20.00	ng/ul	0.00
83) Perylene-d12	23.69	264	2394855	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.34	96	50560	6.95	ng/uL	0.00
5) Phenol-d5	7.02	99	258933	8.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.18	67	638637	34.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.39	132	691467	29.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	520475	19.62	ng/ul	-0.01
19) Nitrobenzene-d5	9.00	128	449546	44.98	ng/ul	0.00
22) 2-Nitrophenol-d4	9.73	143	524668	50.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.26	165	941501	34.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	19943	0.69	ng/ul	-0.15
43) Dimethylphthalate-d6	13.89	166	3455955	36.85	ng/ul	0.00
46) Acenaphthylene-d8	14.17	160	4075707	36.74	ng/ul	0.00
51) 4-Nitrophenol-d4	14.68	143	129430	9.28	ng/ul	-0.01
57) Fluorene-d10	15.47	176	2898051	36.51	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.60	200	539429	44.49	ng/ul	-0.01
70) Anthracene-d10	17.32	188	4686413	39.25	ng/ul	0.00
76) Pyrene-d10	19.62	212	5000542	43.21	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.54	264	4549163	39.98	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
20) Nitrobenzene	9.03	77	34753	1.21	ng/ul#	18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM103117\
Data File : BM012620.D
Acq On : 01 Nov 2017 01:20
Operator : SJ/JU
Sample : I6150-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 01 05:29:16 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 01 05:26:13 2017
Response via : Initial Calibration

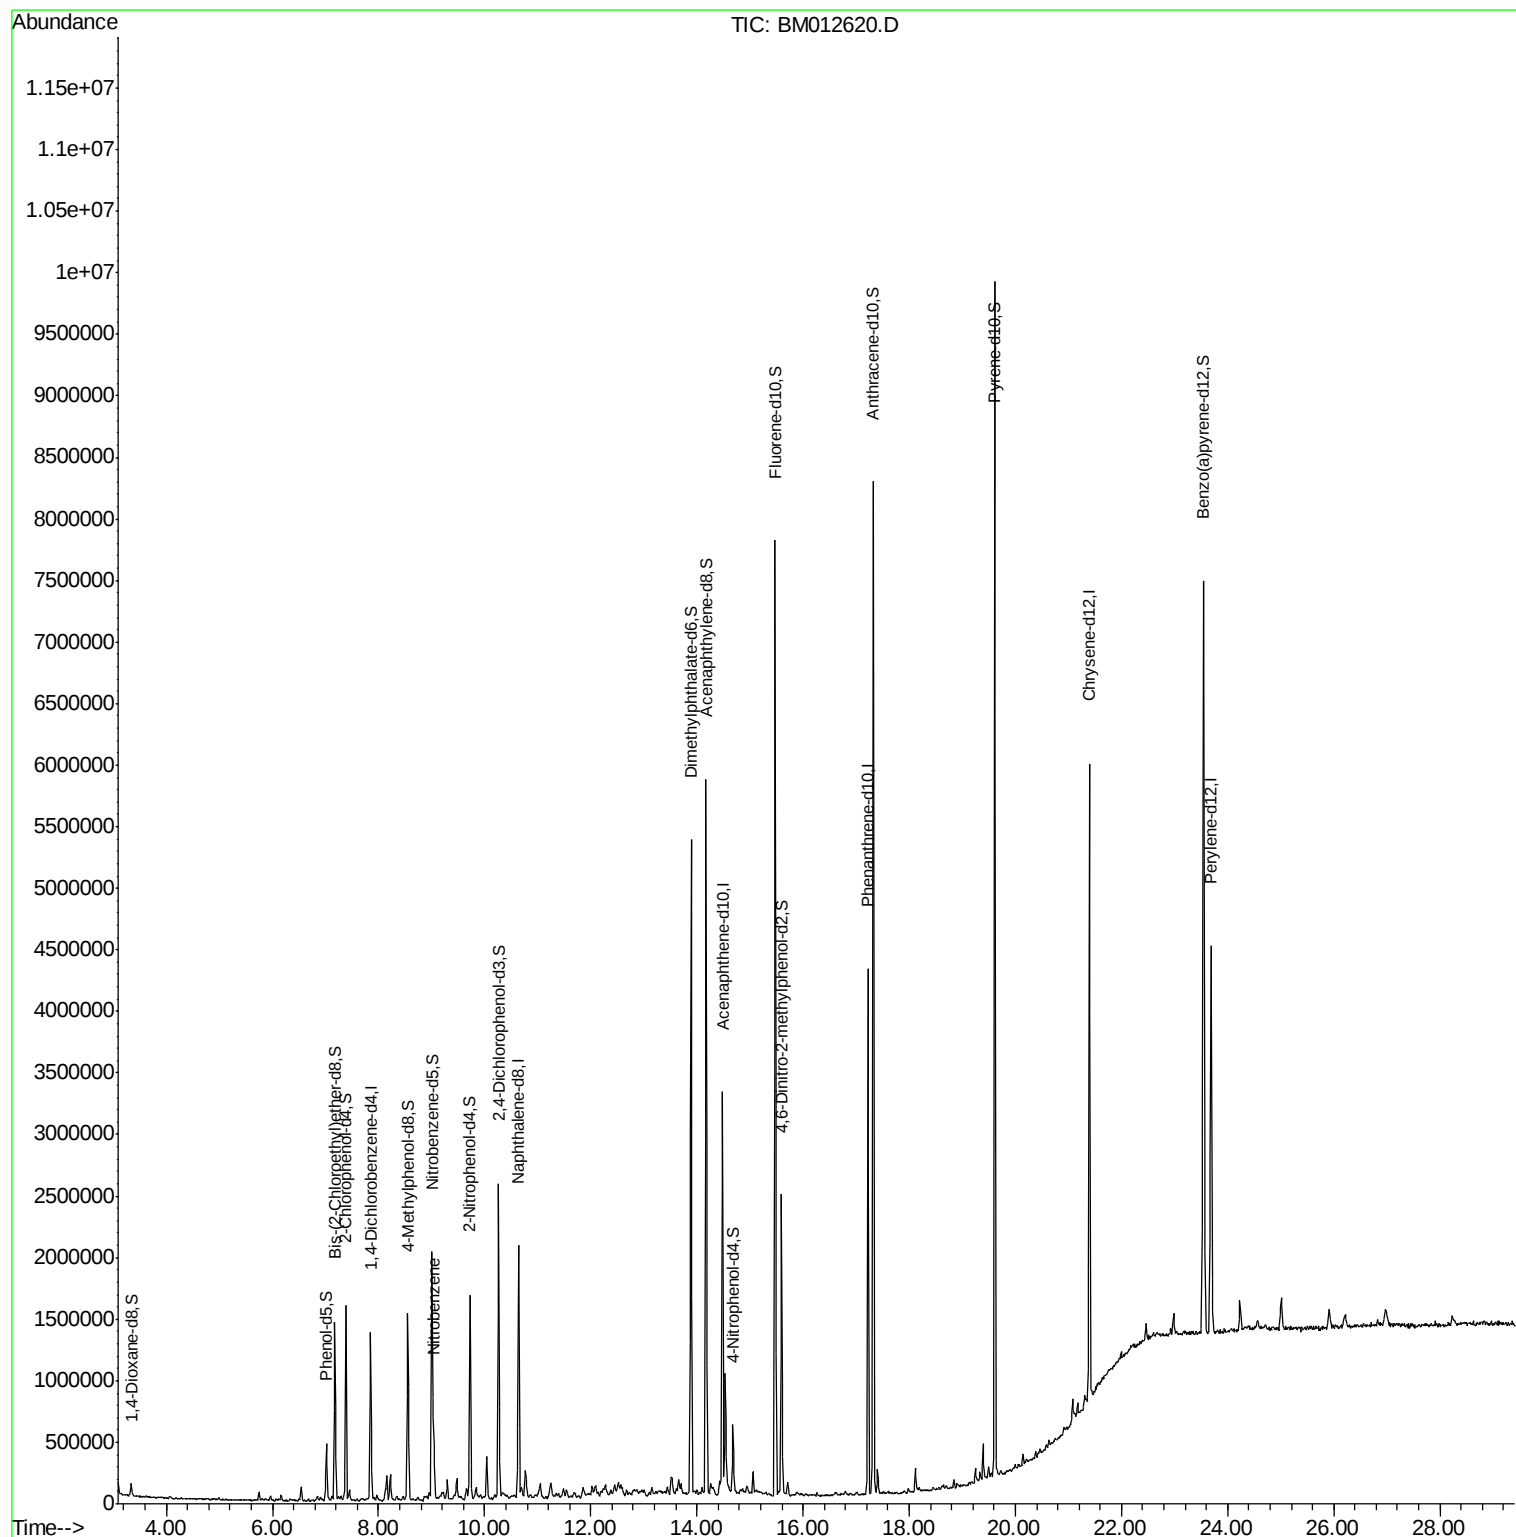

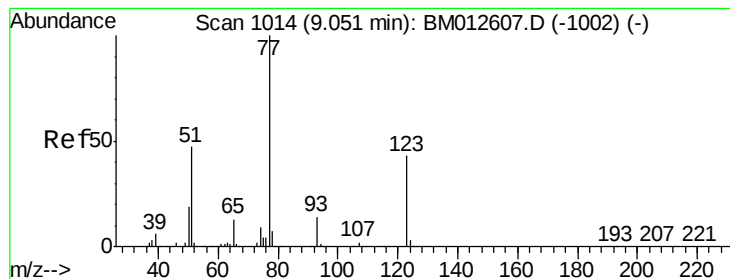

#20

Nitrobenzene

Concen: 1.21 ng/ul

RT: 9.03 min Scan# 1011

Delta R.T. -0.02 min

Lab File: BM012620.D

Acq: 01 Nov 2017 01:20

Instrument :

BNA_M

ClientSampleId :

Tot Ion: 77 Resp: 34753

Ion Ratio Lower Upper

77 100

123 0.0 31.0 46.6#

65 69.6 12.2 18.2#

