
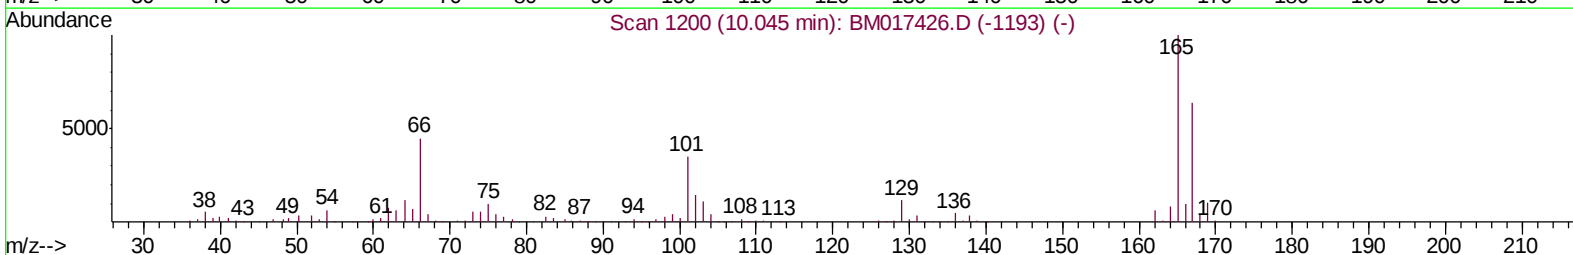
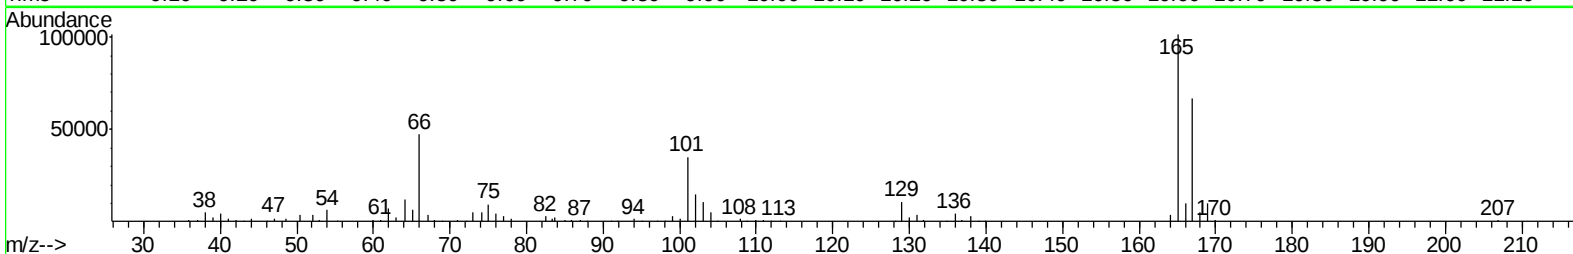


Data File : BM017432.D
Acq On : 31 Oct 2018 16:32
Operator : MJ/SJ
Sample : PB114257BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Nov 01 05:40:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 01 05:28:44 2018
Response via : Initial Calibration

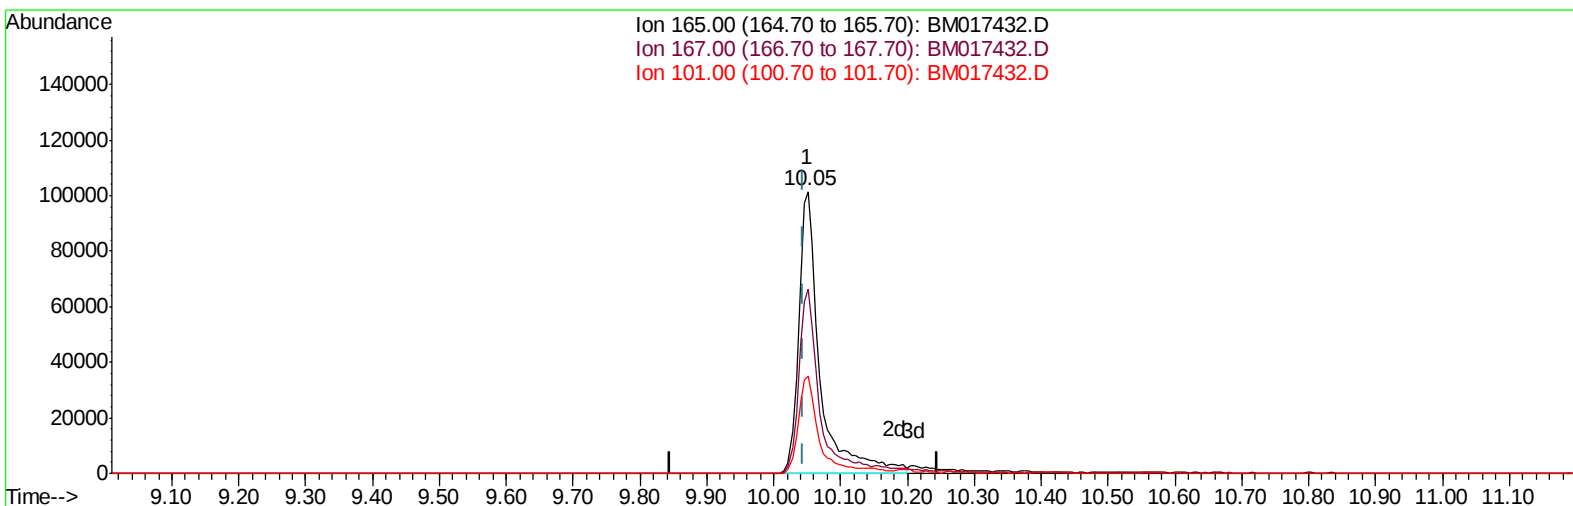

TIC: BM017432.D

(26) 2,4-Dichlorophenol-d3 (S)
10.051min (+0.006) 15.60ng/ul m

response 225581

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	65.63
101.00	34.30	34.67
0.00	0.00	0.00