
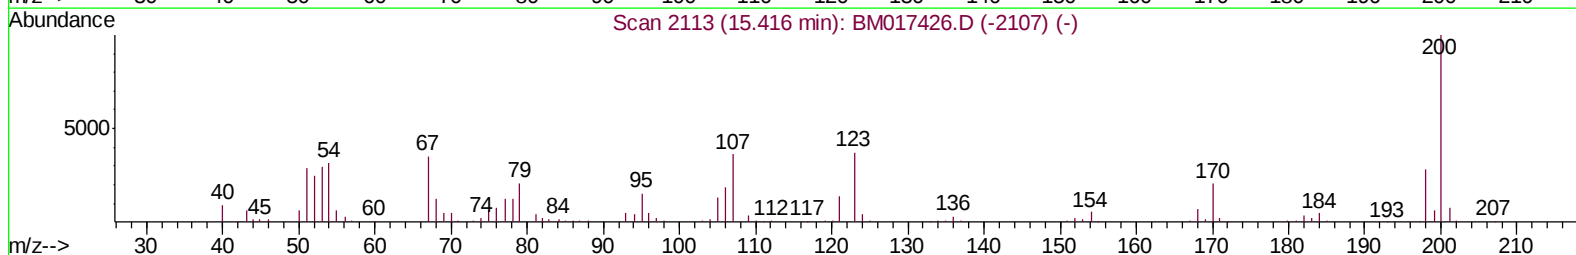
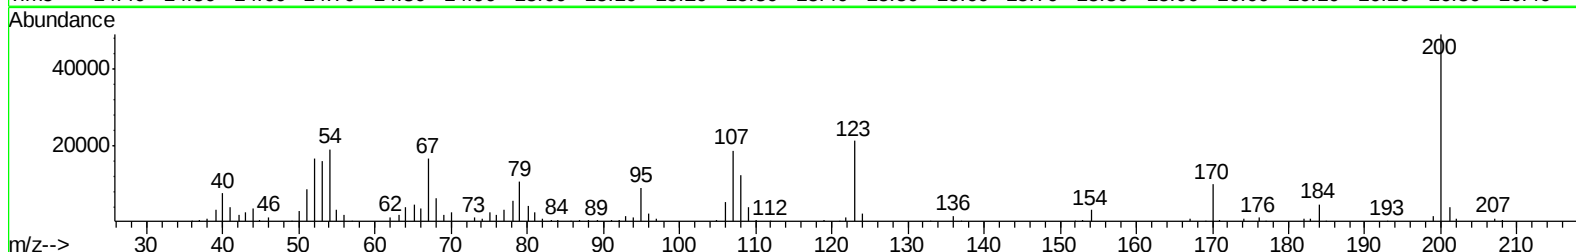


Data File : BM017432.D
Acq On : 31 Oct 2018 16:32
Operator : MJ/SJ
Sample : PB114257BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Nov 01 05:40:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 01 05:28:44 2018
Response via : Initial Calibration

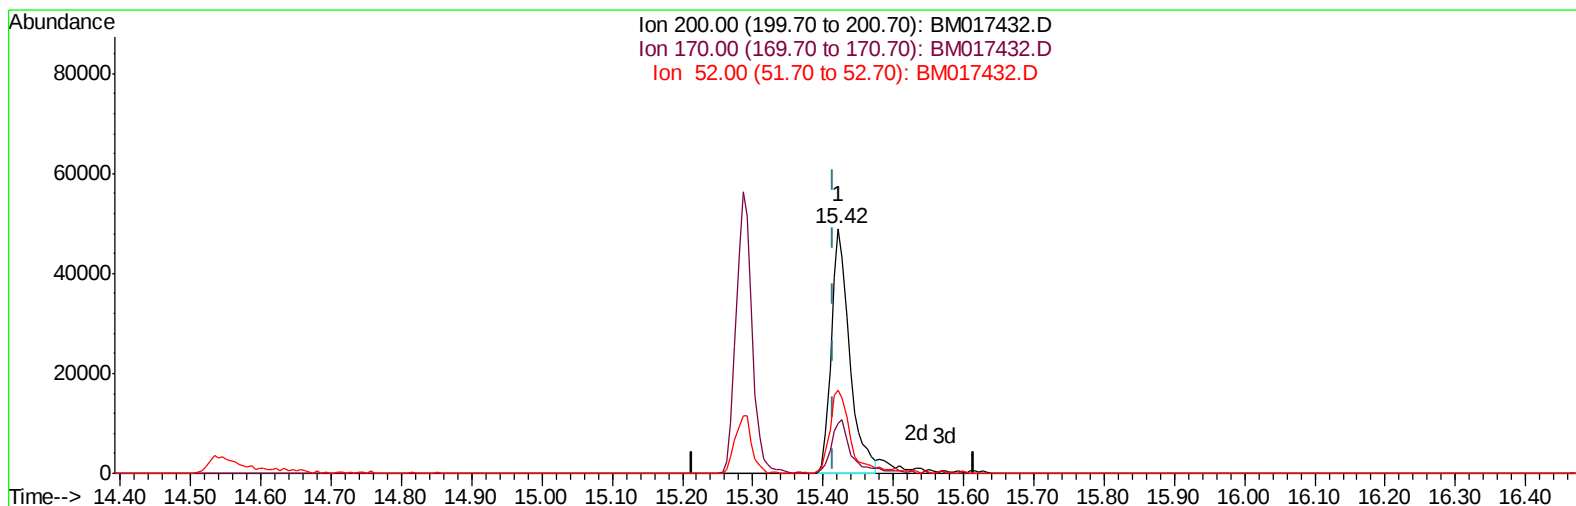

TIC: BM017432.D

(63) 4,6-Dinitro-2-methylphenol-d2 (S)

15.421min (+0.006) 9.58ng/ul

response 88272

Ion	Exp%	Act%
200.00	100	100
170.00	21.00	20.31
52.00	42.60	34.16
0.00	0.00	0.00