
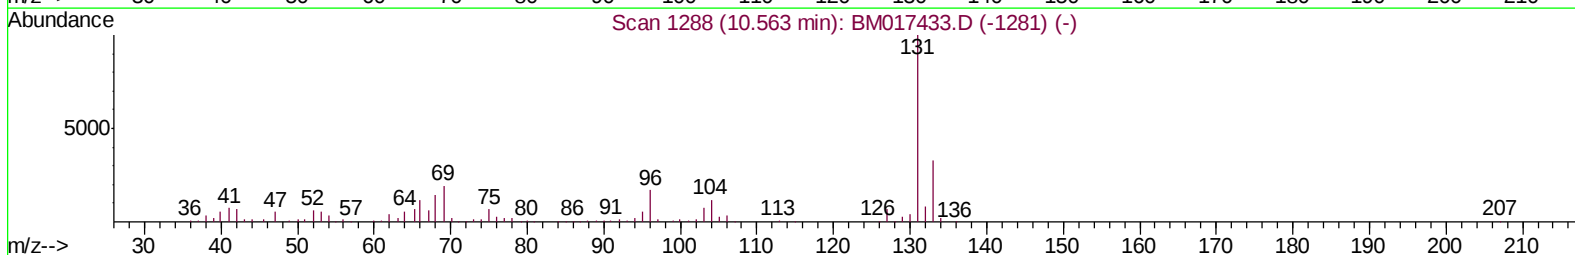
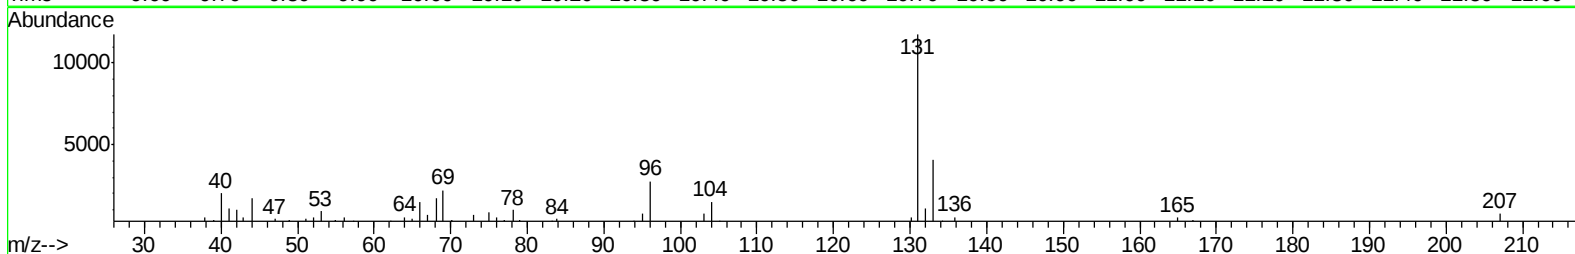


Data File : BM017437.D
Acq On : 31 Oct 2018 19:36
Operator : MJ/SJ
Sample : J5701-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Nov 01 06:49:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 01 06:46:30 2018
Response via : Initial Calibration

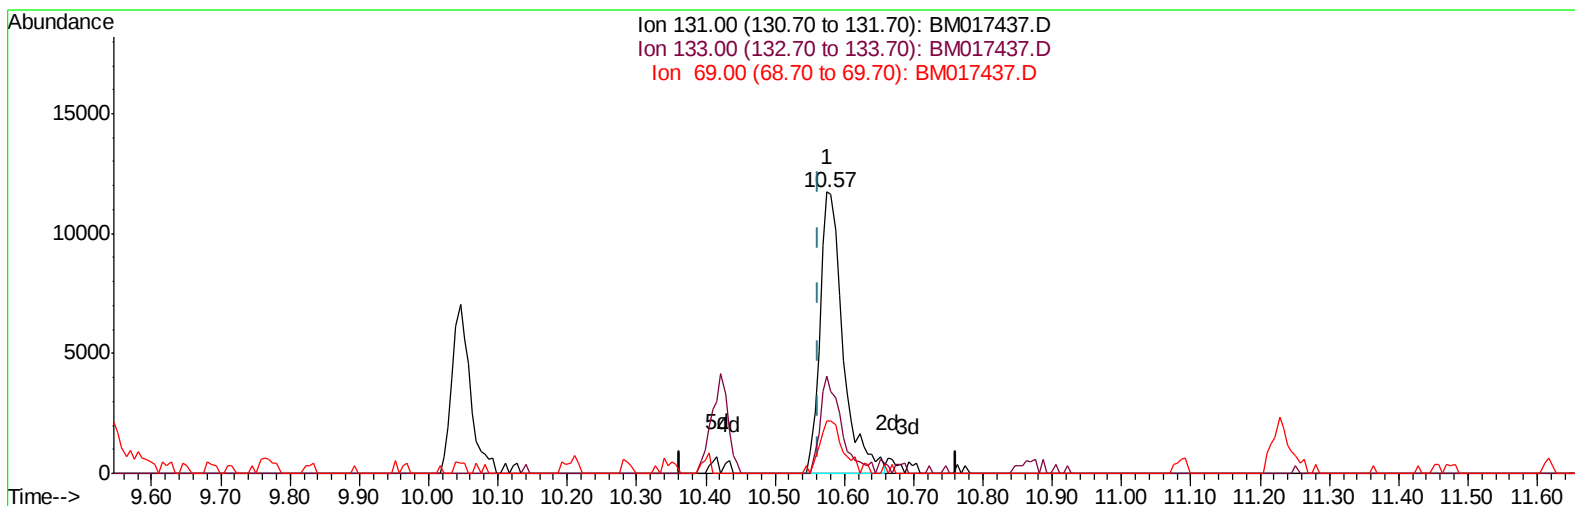

TIC: BM017437.D

(29) 4-Chloroaniline-d4 (S)

10.575min (+0.012) 2.22ng/ul m

response 26930

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	34.62
69.00	17.60	18.68
0.00	0.00	0.00