
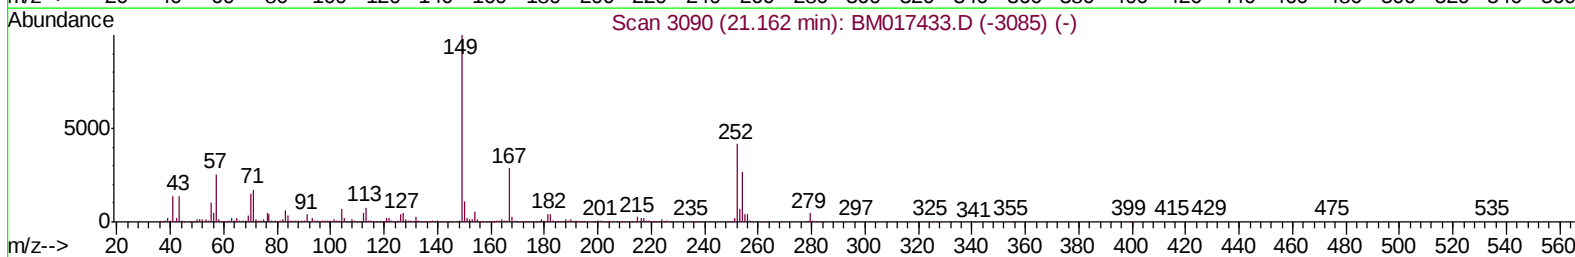
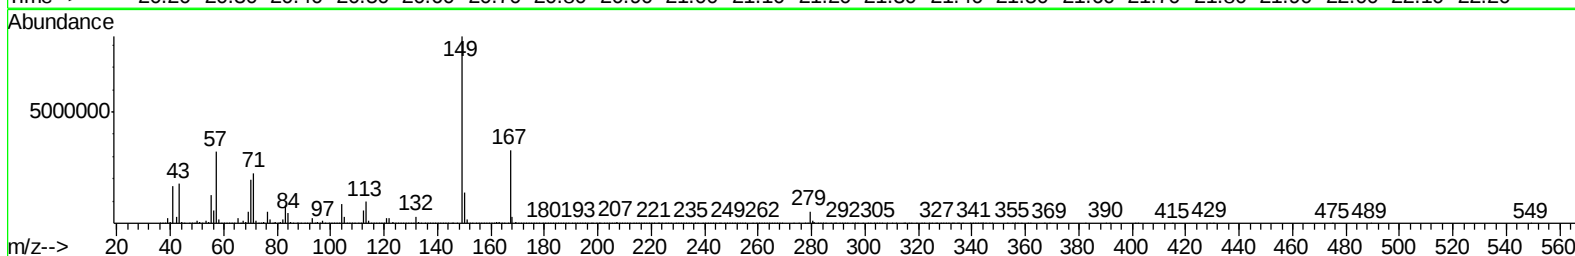


Data File : BM017441.D
Acq On : 31 Oct 2018 22:04
Operator : MJ/SJ
Sample : J5701-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 01 07:19:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 01 06:46:30 2018
Response via : Initial Calibration

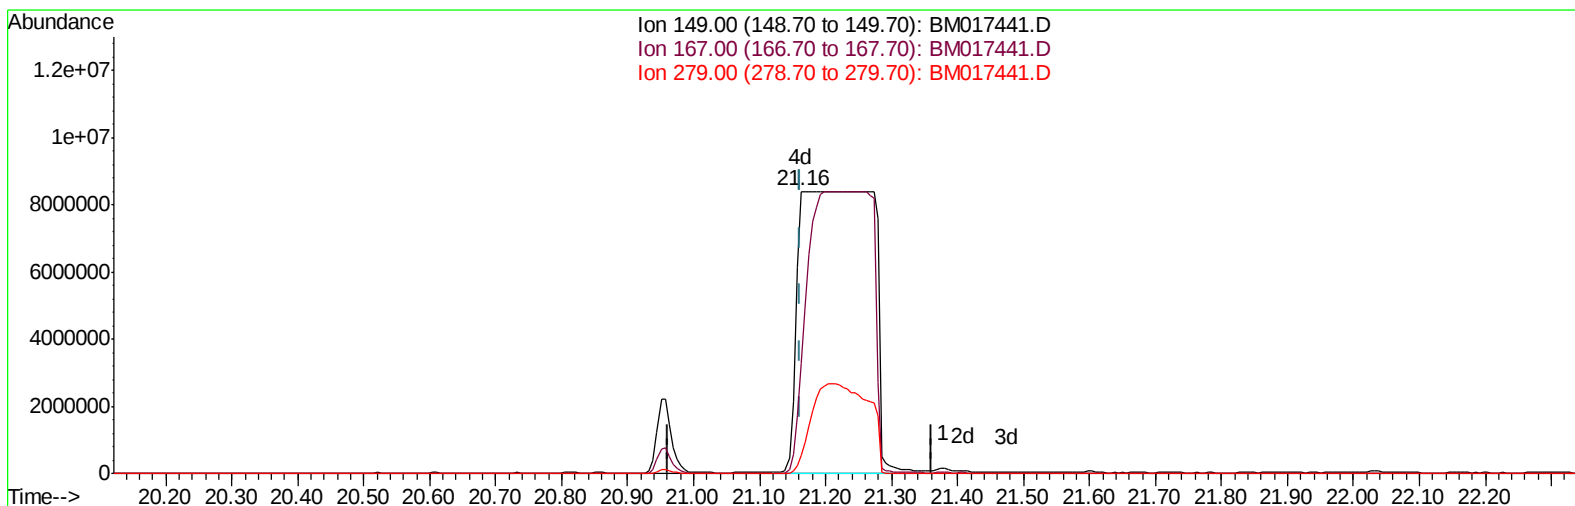

TIC: BM017441.D

(84) Bis(2-ethylhexyl)phthalate

21.162min (-0.000) 3747.71ng/ul m

response 65689849

Ion	Exp%	Act%
149.00	100	100
167.00	28.80	39.16#
279.00	5.10	6.34#
0.00	0.00	0.00