
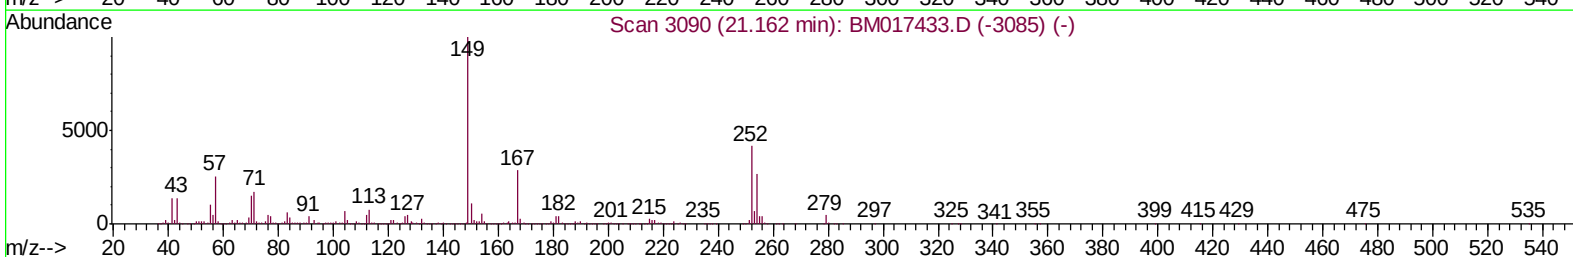
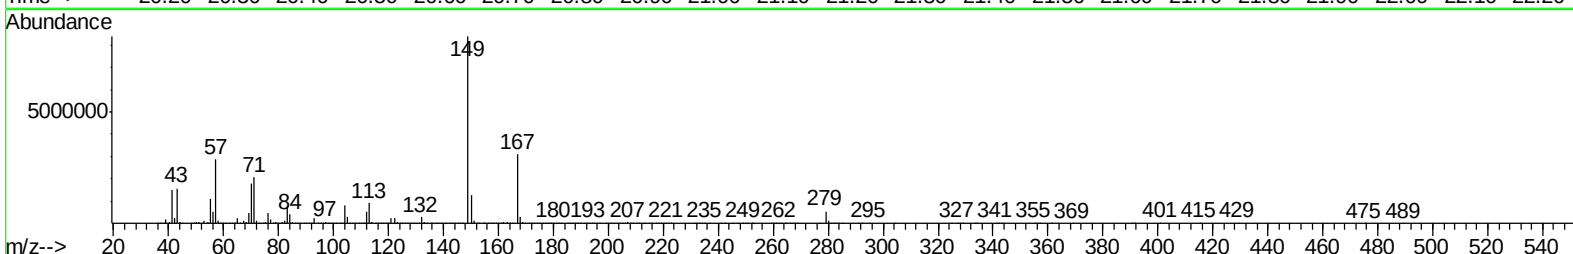


Data File : BM017447.D
Acq On : 01 Nov 2018 01:43
Operator : MJ/SJ
Sample : J5701-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Nov 01 06:50:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 01 06:46:30 2018
Response via : Initial Calibration

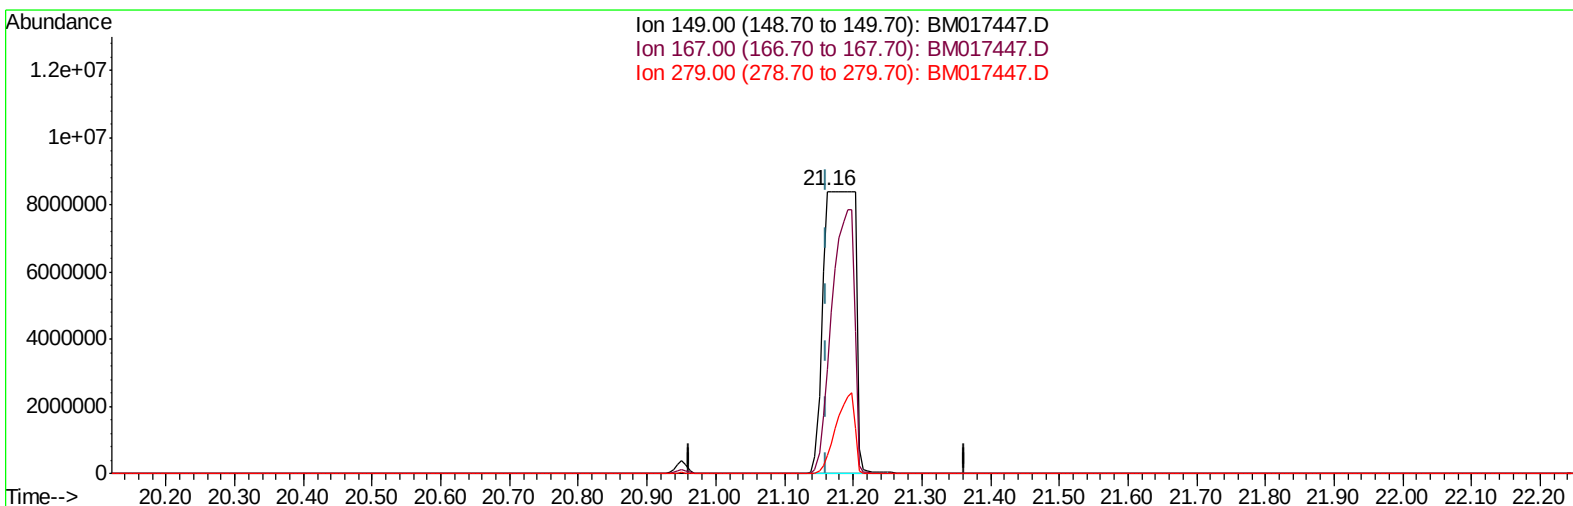

TIC: BM017447.D

(84) Bis(2-ethylhexyl)phthalate

21.162min (-0.000) 398.88ng/ul m

response 27203852

Ion	Exp%	Act%
149.00	100	100
167.00	28.80	36.92#
279.00	5.10	6.17#
0.00	0.00	0.00