

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM103118\
Quantitation Report (QT Reviewed)


Data File : BM017451.D
Acq On : 01 Nov 2018 04:09
Operator : MJ/SJ
Sample : J5701-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40E9

Manual Integrations
APPROVED

Sohil
11/1/2018 10:55:33 AM

Quant Time: Nov 01 08:04:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 01 07:49:12 2018
Response via : Initial Calibration

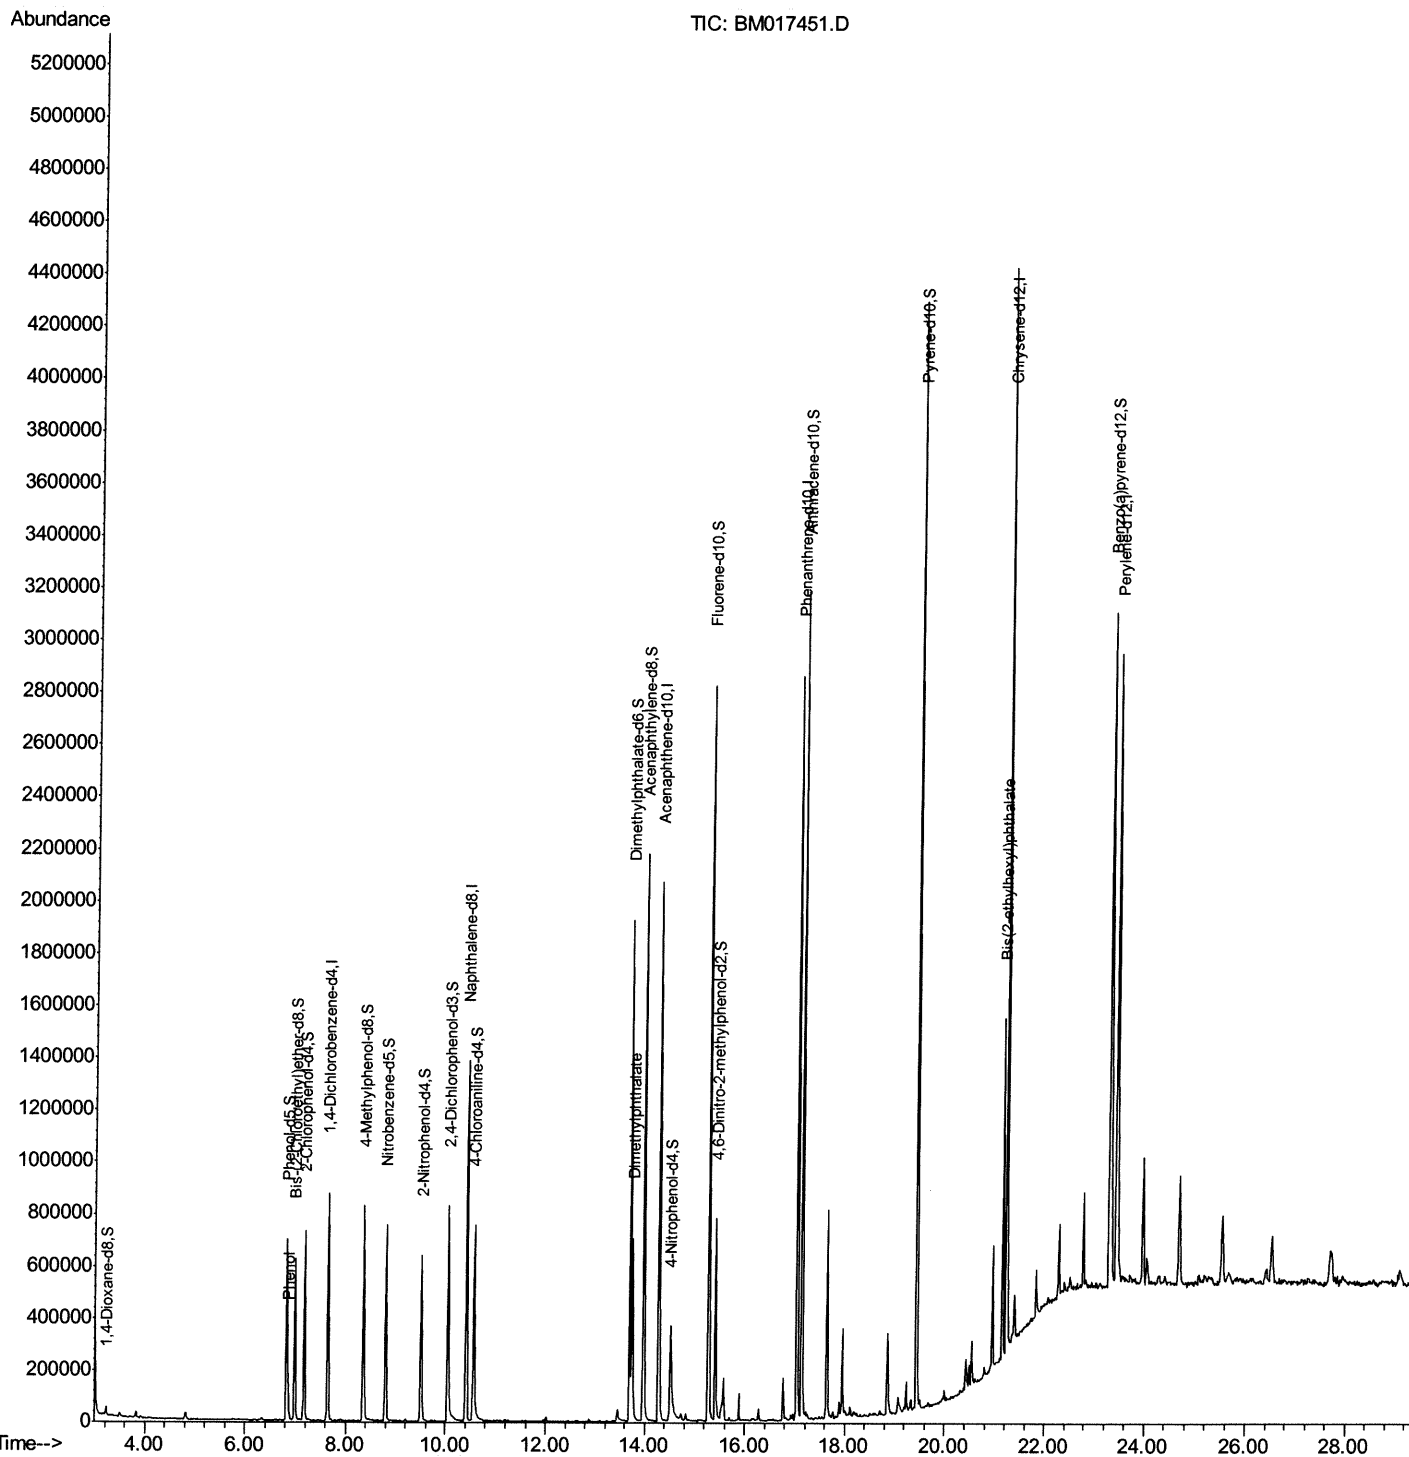

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM103118\
Quantitation Report (Qedit)




Data File : BM017451.D
Acq On : 01 Nov 2018 04:09
Operator : MJ/SJ
Sample : J5701-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40E9

Manual Integrations
APPROVED

Sohil
11/1/2018 10:55:33 AM

Quant Time: Nov 01 07:51:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 01 07:49:12 2018
Response via : Initial Calibration

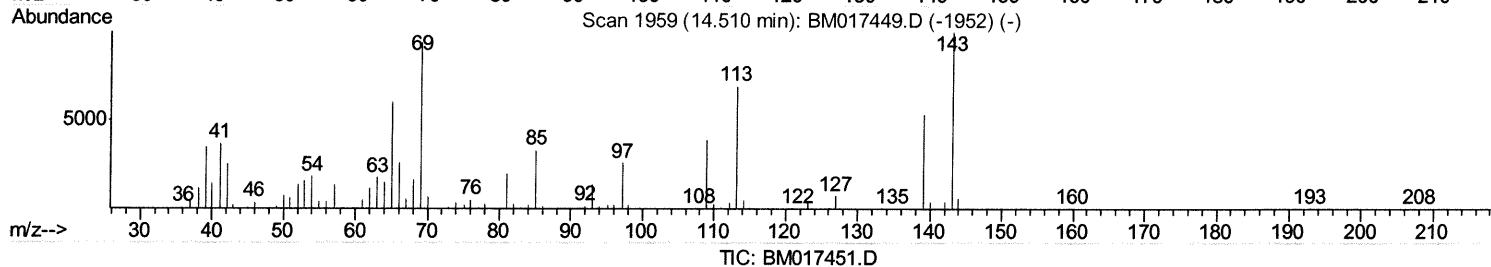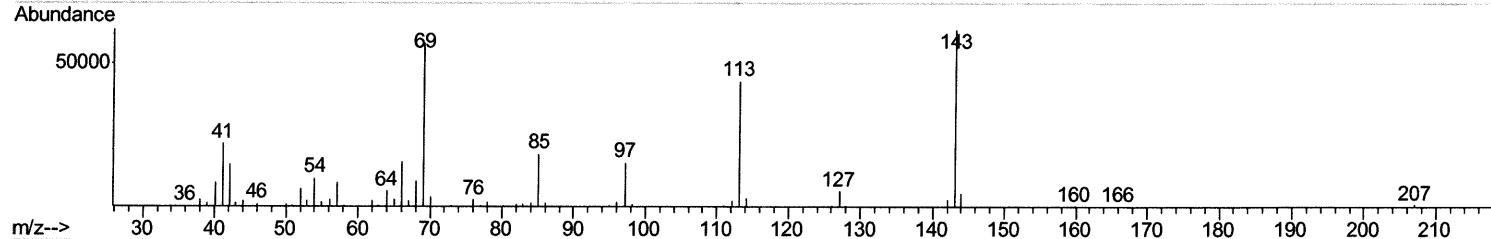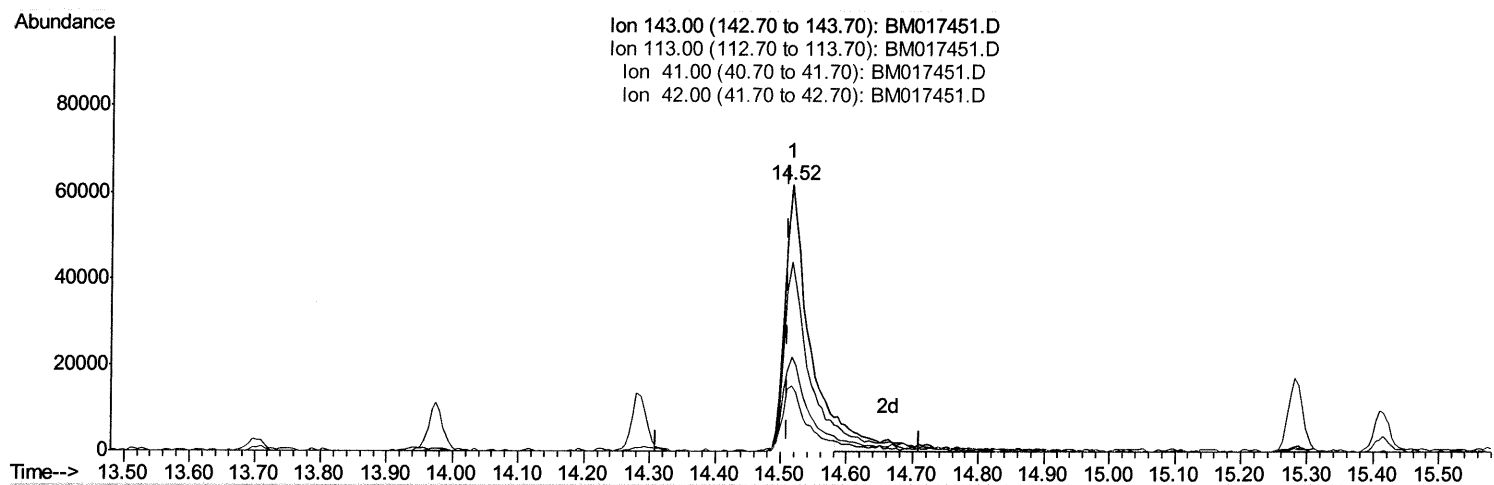

(52) 4-Nitrophenol-d4 (S)

14.516min (+0.006) 12.67ng/ul

response 146990

Ion	Exp%	Act%
143.00	100	100
113.00	74.20	70.84
41.00	39.30	35.65
42.00	25.10	24.64

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM103118\
Quantitation Report (Qedit)




Data File : BM017451.D
Acq On : 01 Nov 2018 04:09
Operator : MJ/SJ
Sample : J5701-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40E9

Manual Integrations
APPROVED

Sohil
11/1/2018 10:55:33 AM

Quant Time: Nov 01 07:51:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 01 07:49:12 2018
Response via : Initial Calibration

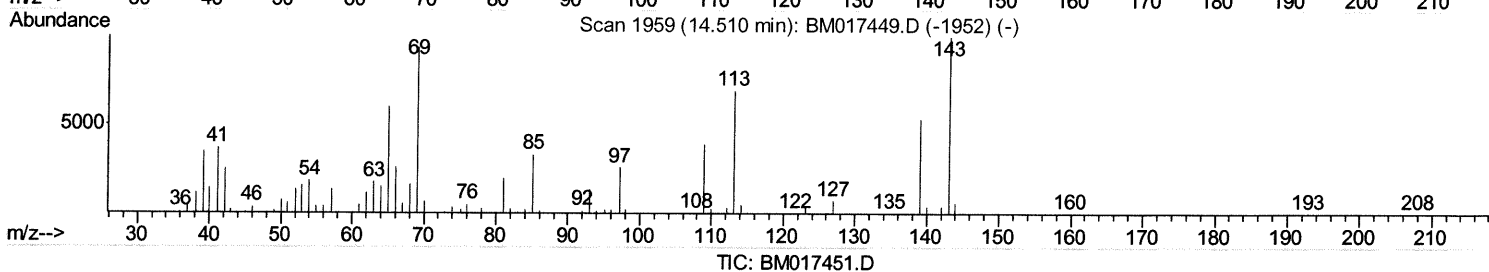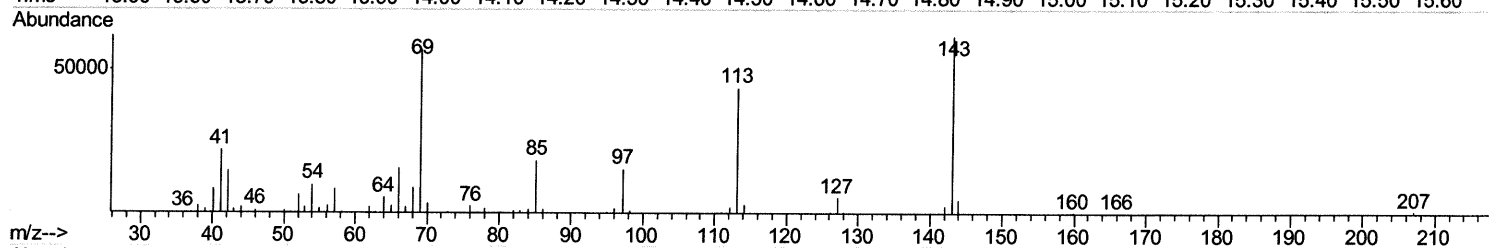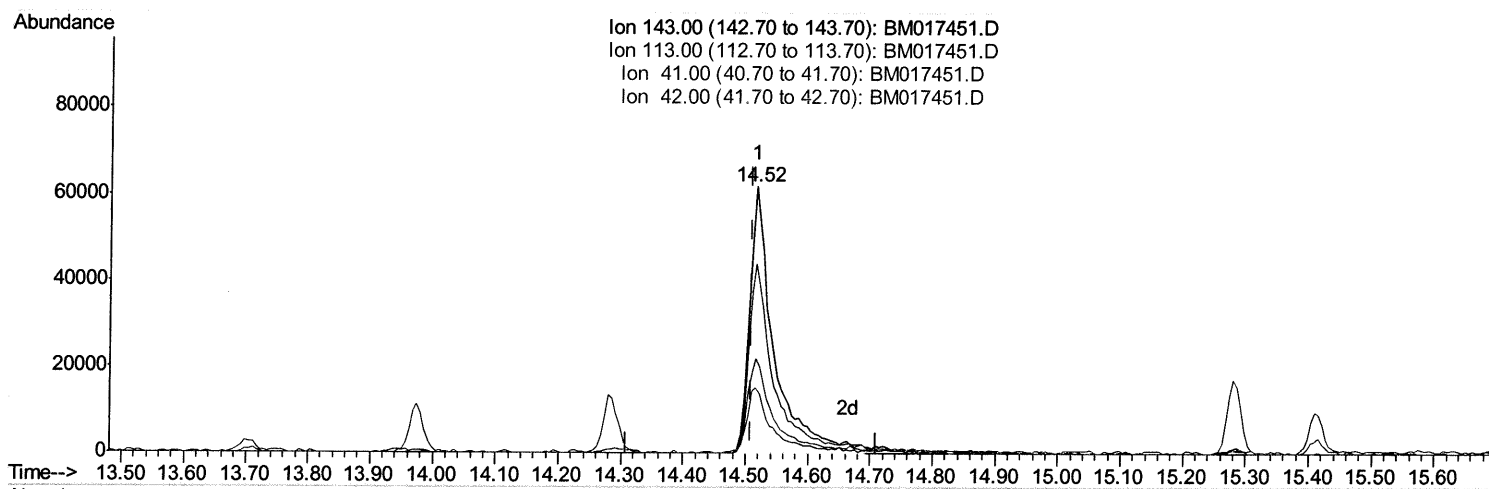

(52) 4-Nitrophenol-d4 (S)

14.516min (+0.006) 14.70ng/ul m

response 170515

Ion	Exp%	Act%
143.00	100	100
113.00	74.20	70.84
41.00	39.30	35.65
42.00	25.10	24.64

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM103118\
Quantitation Report (QT Reviewed)

Data File : BM017451.D
Acq On : 01 Nov 2018 04:09
Operator : MJ/SJ
Sample : J5701-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40E9

Manual Integrations
APPROVED

Sohil
11/1/2018 10:55:33 AM

Quant Time: Nov 01 08:04:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 01 07:49:12 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	241356	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1152588	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	724135	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	1734788	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	1908721	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	1769360	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	19652	3.75	ng/uL	0.00
5) Phenol-d5	6.82	99	411601	18.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	277530	21.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	353759	20.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	332883	19.10	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	189821	21.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	210911	20.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	362228	19.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	465261	30.37	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	1372654	22.10	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	1626113	21.57	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	170515m	14.70	ng/ul	0.00
58) Fluorene-d10	15.29	176	1197736	22.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	188593	15.60	ng/ul	0.00
71) Anthracene-d10	17.13	188	1860395	21.66	ng/ul	0.00
79) Pyrene-d10	19.44	212	2075645	23.47	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	1983268	21.22	ng/ul	0.00

5/11/2/18

Target Compounds					Qvalue
6) Phenol	6.85	94	77205	3.527	ng/ul 98
45) Dimethylphthalate	13.75	163	456158	7.582	ng/ul 100
84) Bis(2-ethylhexyl)phthalate	21.16	149	416122	6.435	ng/ul# 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed