

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103118\
 Data File : BM017454.D
 Acq On : 01 Nov 2018 05:58
 Operator : MJ/SJ
 Sample : J5701-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40F9

Manual Integrations
 APPROVED

Sohil
 11/1/2018 10:55:38 AM

Quant Time: Nov 01 08:20:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 01 07:49:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	300780	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1360420	20.00	ng/ul	0.01
36) Acenaphthene-d10	14.29	164	784959	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.09	188	5859937m	20.00	ng/ul	0.05
78) Chrysene-d12	21.24	240	2074317	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	1996715	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	15444	2.36	ng/uL	0.00
5) Phenol-d5	6.82	99	383235	13.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	255404	15.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	332894	15.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	343403	15.81	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	182934	17.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	203625	17.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	334450	15.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	453945	25.11	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	1267955	18.84	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	1563664	19.13	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	138851	11.04	ng/ul	0.00
58) Fluorene-d10	15.29	176	1051401	17.98	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	160906	3.94	ng/ul	0.00
71) Anthracene-d10	17.17	188	1763616	6.08	ng/ul	0.03
79) Pyrene-d10	19.47	212	2026057	21.08	ng/ul	0.03
90) Benzo(a)pyrene-d12	23.30	264	1821973	17.28	ng/ul	0.00

Target Compounds

					Ovalue	
6) Phenol	6.85	94	108778	3.987	ng/ul	97
37) 1,2,4,5-Tetrachlorobenzene	12.46	216	68950	2.614	ng/ul#	95
45) Dimethylphthalate	13.75	163	406434	6.232	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	21.16	149	12627370	179.697	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103118\
Data File : BM017454.D
Acq On : 01 Nov 2018 05:58
Operator : MJ/SJ
Sample : J5701-12
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A40F9

Quant Time: Nov 01 08:20:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 01 07:49:12 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
11/1/2018 10:55:38 AM

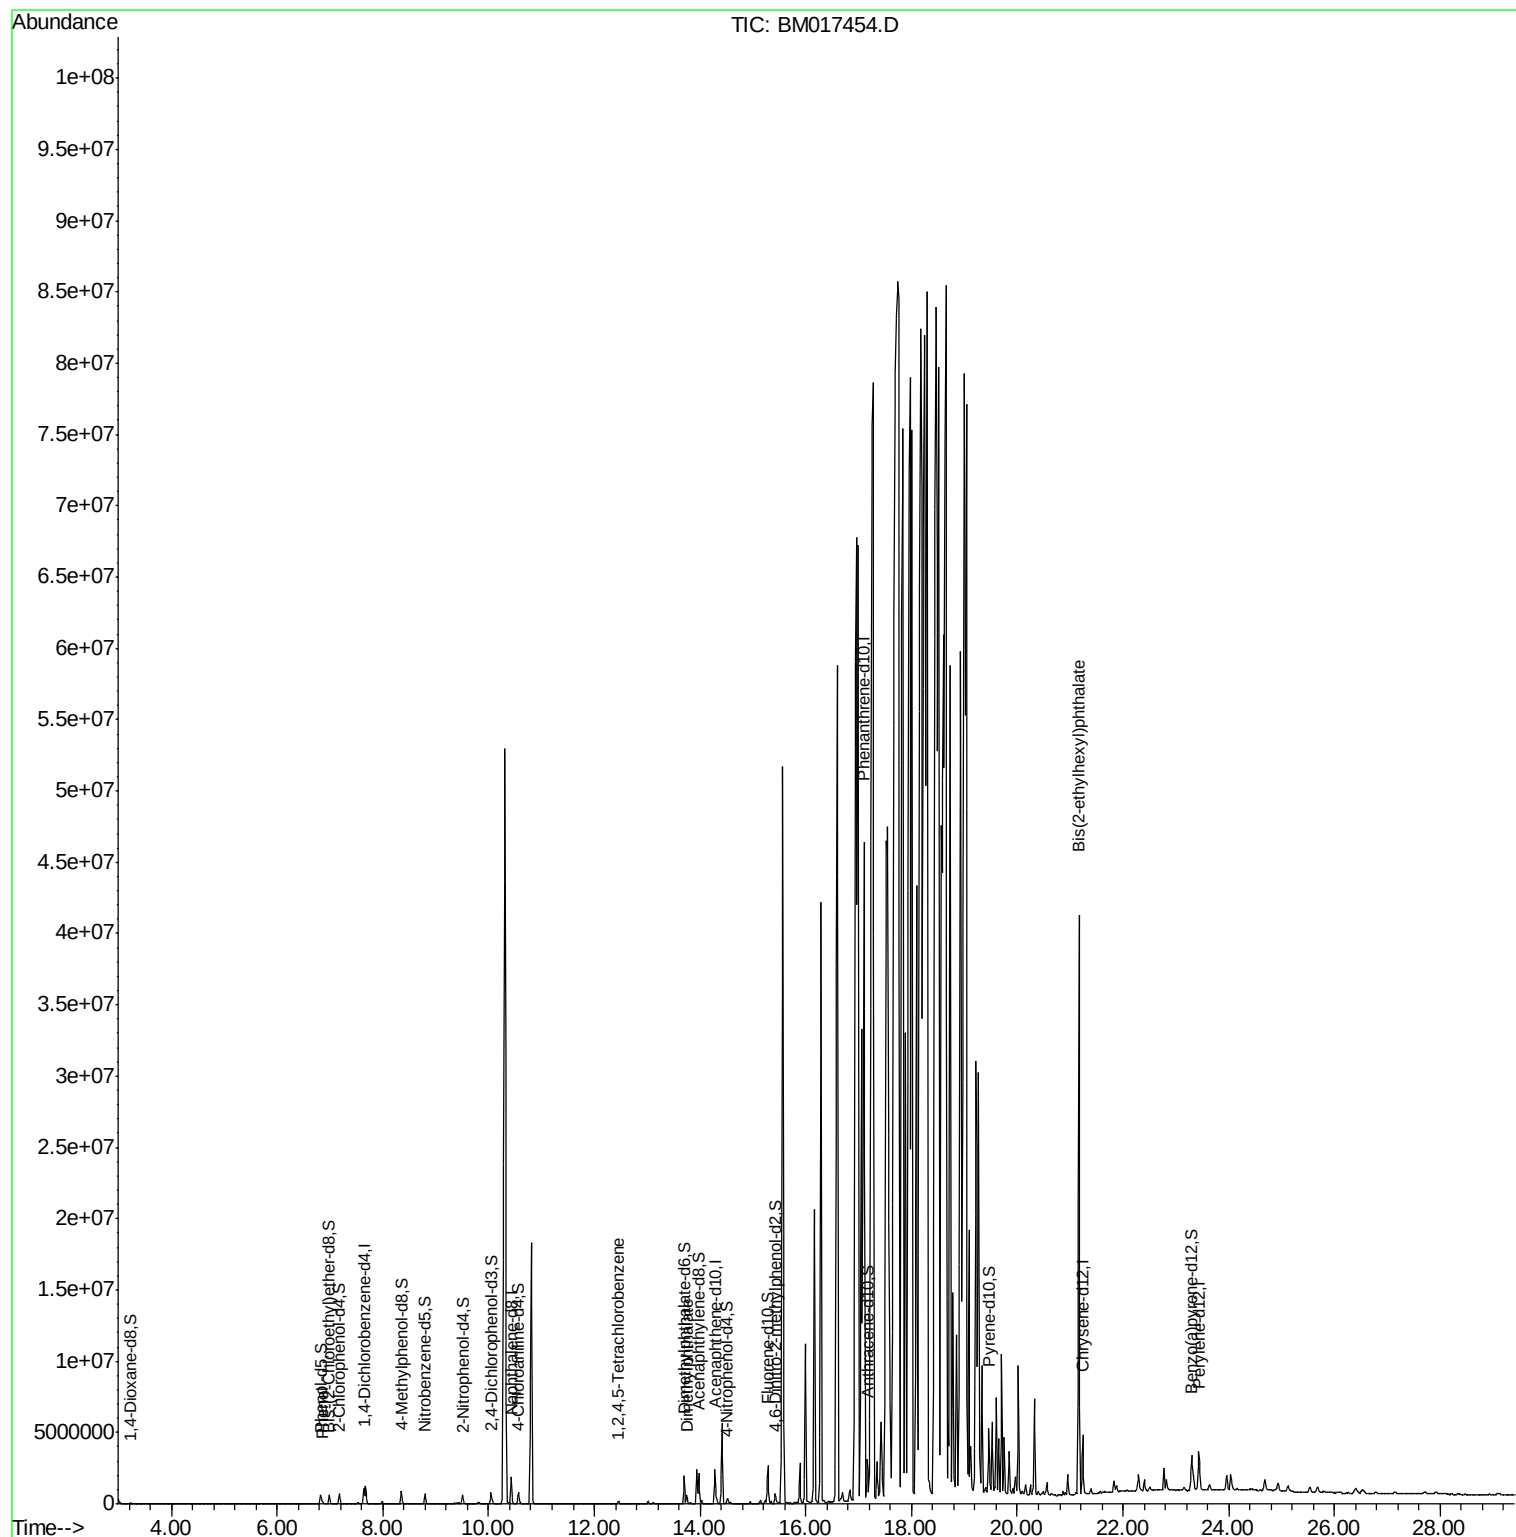

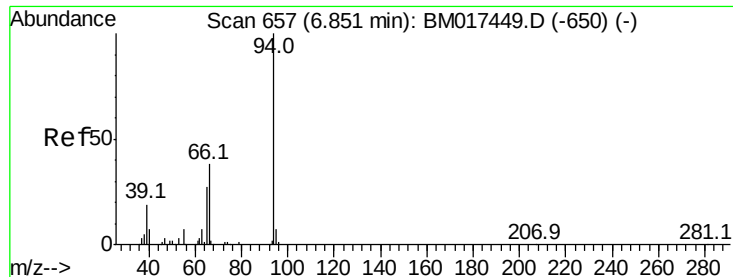

#6

Phenol

Concen: 3.987 ng/ul

RT: 6.85 min Scan# 657

Delta R.T. 0.00 min

Lab File: BM017454.D

Acq: 01 Nov 2018 05:58

Instrument :

BNA_M

ClientSampleId :

A40F9

Tot Ion: 94 Resp: 108778

Ion Ratio Lower Upper

94 100

65 27.4 24.0 36.0





66 38.4 31.1 46.7

Manual Integrations

APPROVED

Sohil

11/1/2018 10:55:38 AM

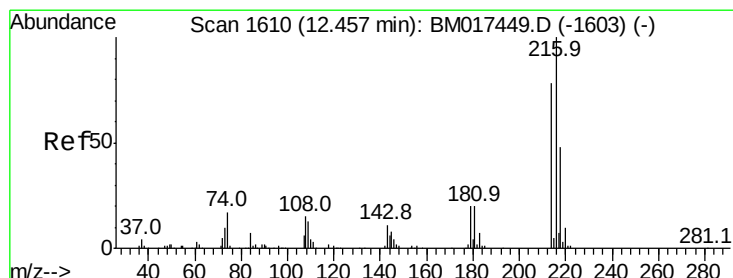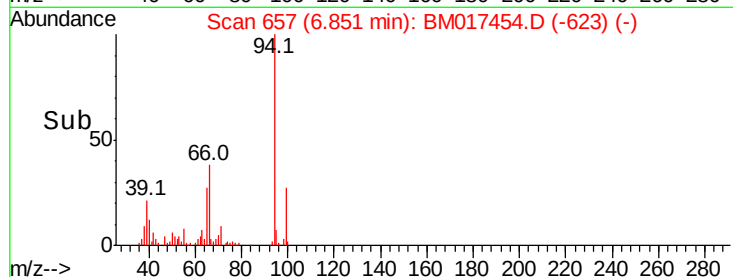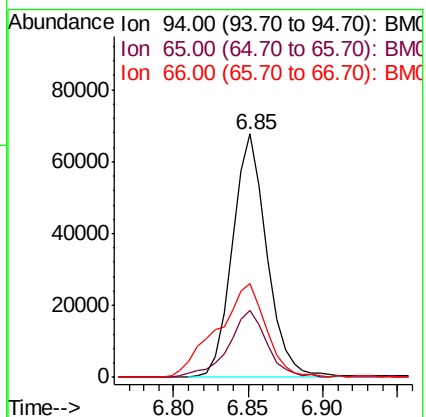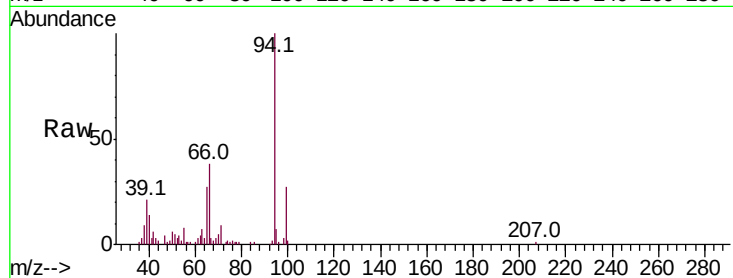

#37

1,2,4,5-Tetrachlorobenzene

Concen: 2.614 ng/ul

RT: 12.46 min Scan# 1611

Delta R.T. 0.01 min

Lab File: BM017454.D

Acq: 01 Nov 2018 05:58

Tgt Ion: 216 Resp: 68950




Ion Ratio Lower Upper


216 100

214 74.2 61.7 92.5

179 16.4 16.0 24.0

108 11.5 12.6 18.8#

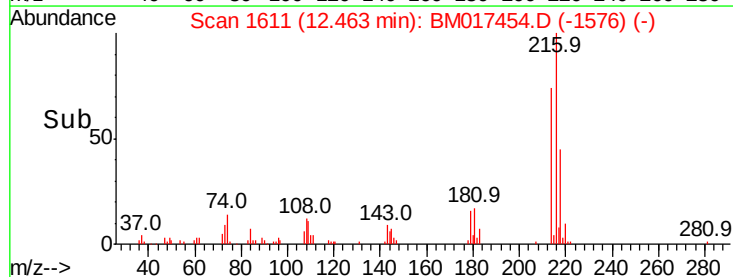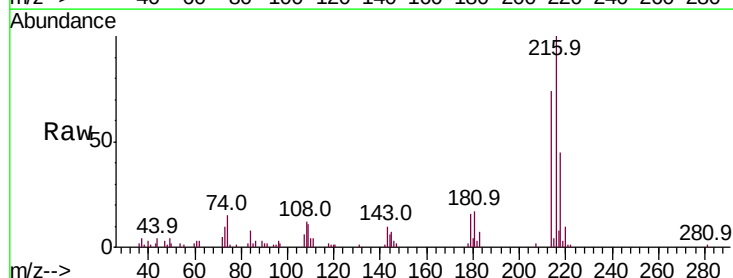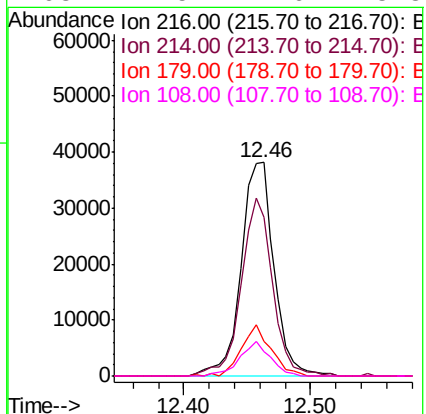

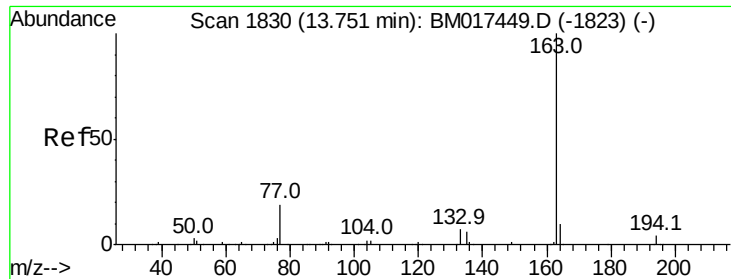


#45
 Dimethylphthalate
 Concen: 6.232 ng/ul
 RT: 13.75 min Scan# 1830
 Delta R.T. 0.00 min
 Lab File: BM017454.D
 Acq: 01 Nov 2018 05:58

Instrument :
 BNA_M
 ClientSampleId :
 A40F9

Tot Ion	Ratio	Resp	Lower	Upper
163	100	406434		
194	4.1	3.2	4.8	
164	10.4	8.1	12.1	

Manual Integrations
 APPROVED

Sohil
 11/1/2018 10:55:38 AM



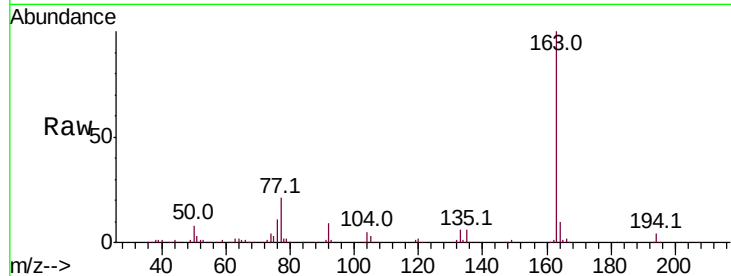


Abundance

Ion 163.00 (162.70 to 163.70): E


Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

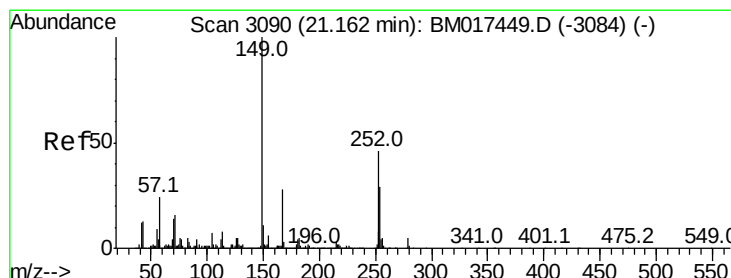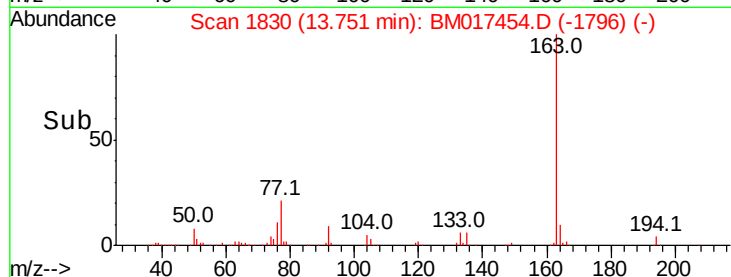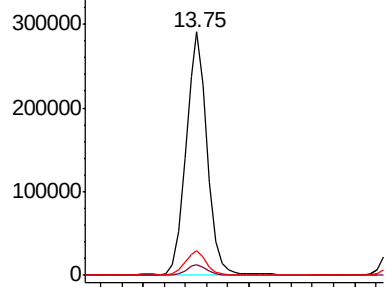

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 179.697 ng/ul
 RT: 21.16 min Scan# 3090
 Delta R.T. 0.00 min
 Lab File: BM017454.D
 Acq: 01 Nov 2018 05:58

Tgt Ion	Ratio	Resp	Lower	Upper
149	100	12627370		
167	36.4	23.0	34.6#	
279	6.1	4.1	6.1	

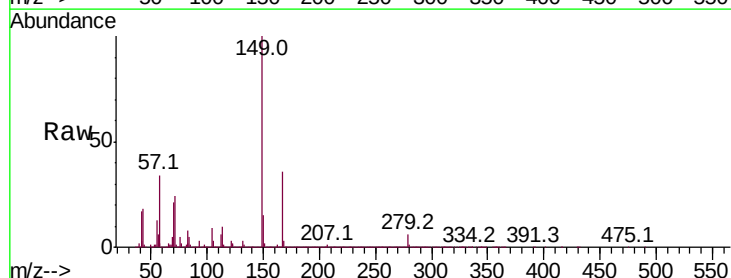

Abundance

Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

