

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
 Data File : BM023548.D
 Acq On : 01 Nov 2019 08:15
 Operator : JU
 Sample : K5433-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 01 10:40:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 01 08:19:37 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	467949	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1903940	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	1152766	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	2430962	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	2377608	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	2787857	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	23129	2.35	ng/uL	0.00
5) Phenol-d5	6.79	99	492553	12.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	300253	13.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	407308	13.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	379806	11.90	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	205679	14.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	218014	13.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	395947	12.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	383652	10.68	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	1228922	14.04	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	1464742	14.61	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	127013	8.38	ng/ul	0.00
58) Fluorene-d10	15.26	176	1064104	14.35	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	108971	7.20	ng/ul	0.00
71) Anthracene-d10	17.10	188	1588681	13.83	ng/ul	0.00
79) Pyrene-d10	19.40	212	1823028	13.94	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	2069822	14.57	ng/ul	-0.01
Target Compounds						
8) Bis(2-Chloroethyl)ether	7.06	93	33630	1.066	ng/ul#	24
45) Dimethylphthalate	13.72	163	397718	4.525	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
Data File : BM023548.D
Acq On : 01 Nov 2019 08:15
Operator : JU
Sample : K5433-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 01 10:40:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 01 08:19:37 2019
Response via : Initial Calibration

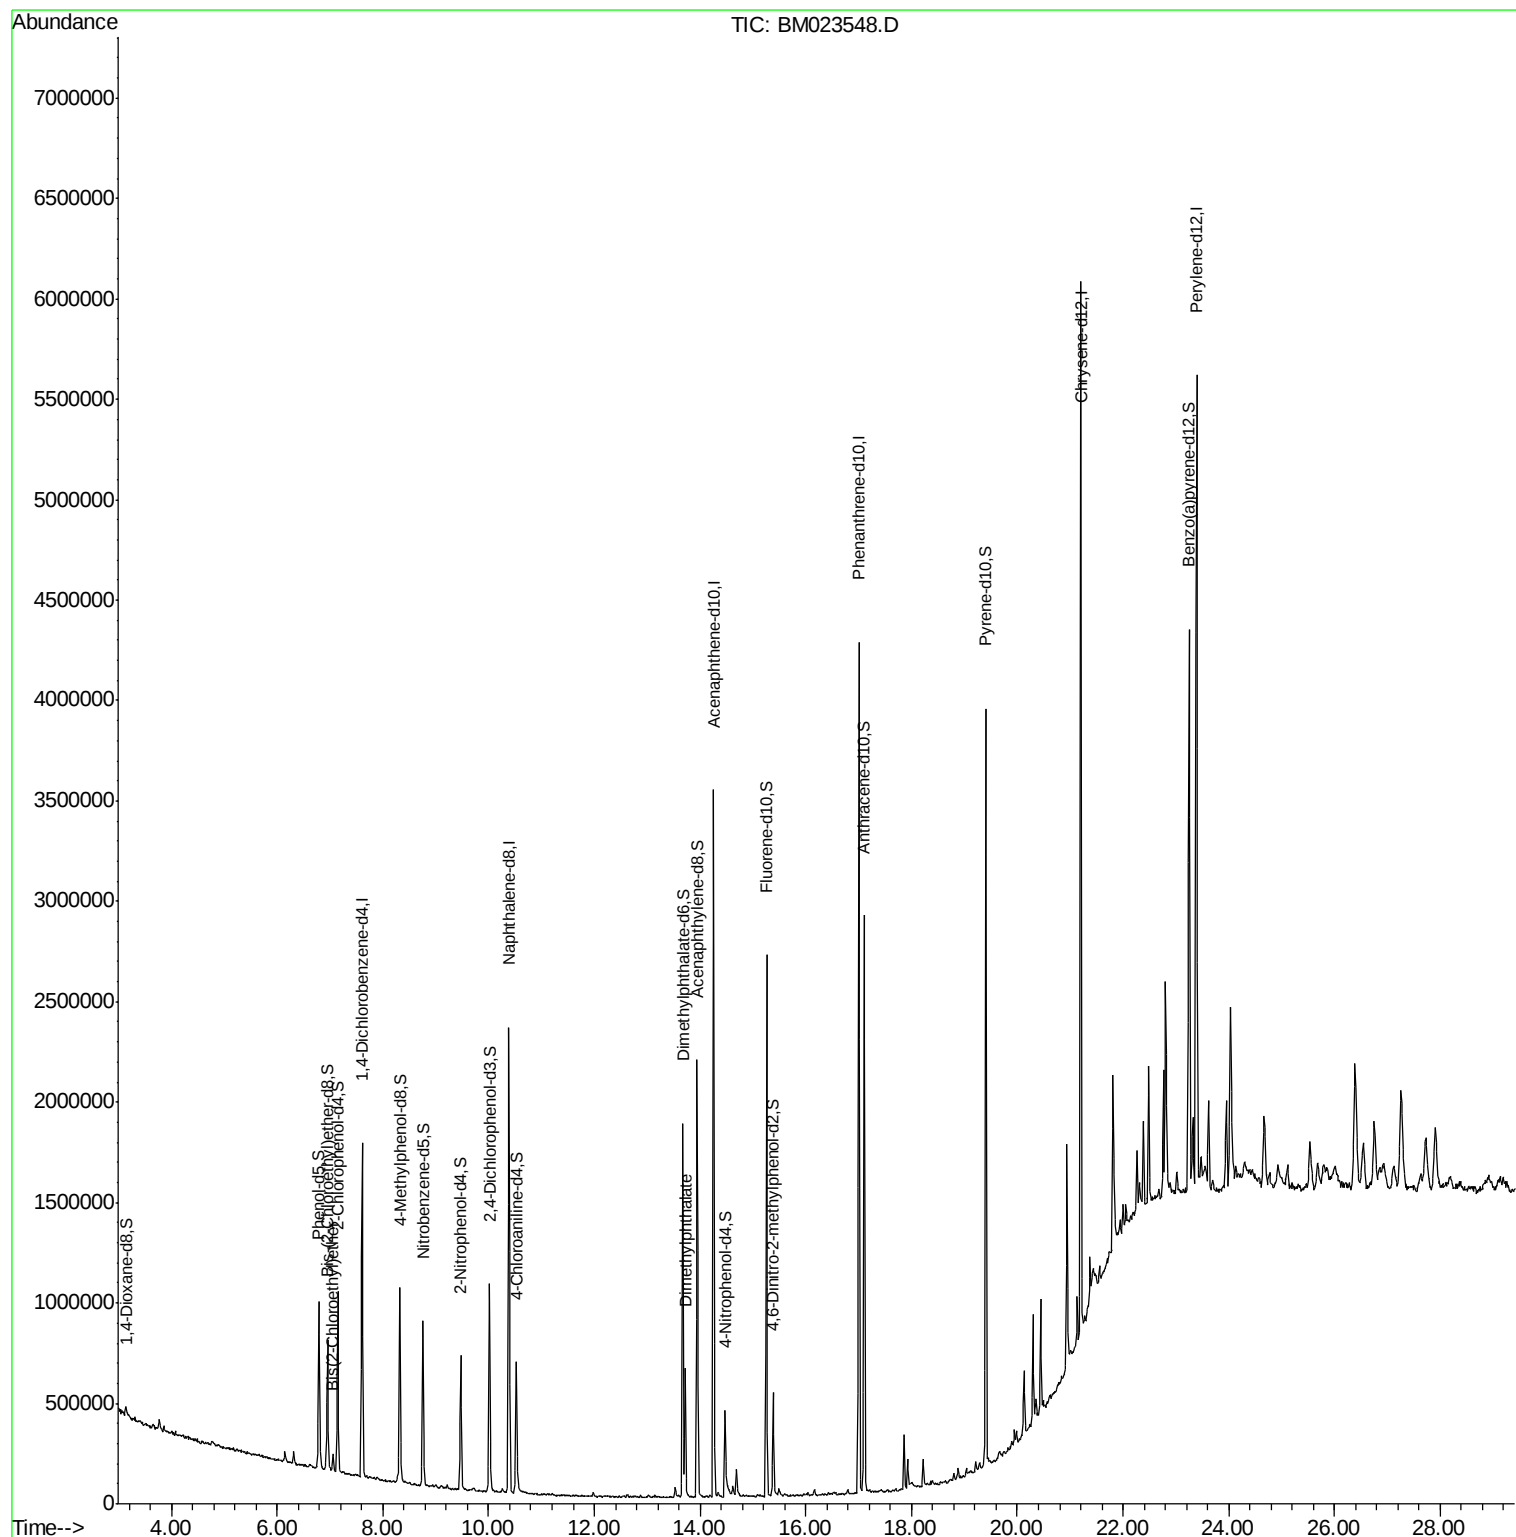




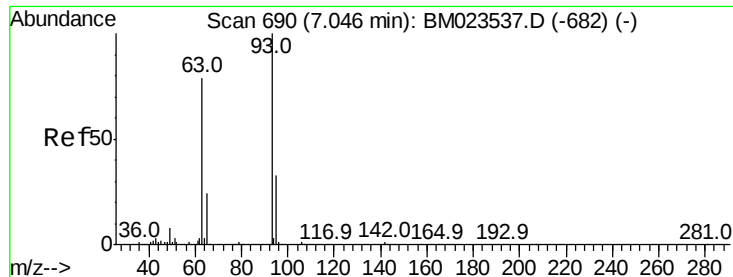


#8

Bis(2-Chloroethyl)ether
 Concen: 1.066 ng/ul
 RT: 7.06 min Scan# 692
 Delta R.T. 0.01 min
 Lab File: BM023548.D
 Acq: 01 Nov 2019 08:15

Instrument :
 BNA_M
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
93	100		
63	1.9	61.4	92.0#
95	4.3	26.1	39.1#

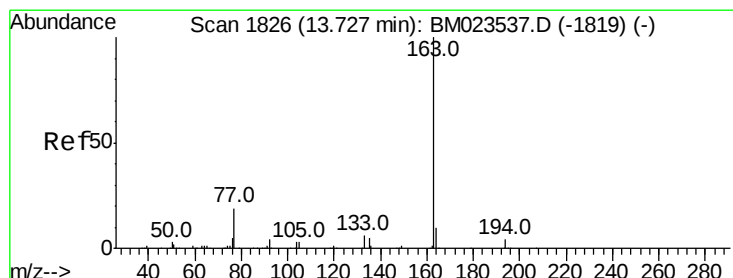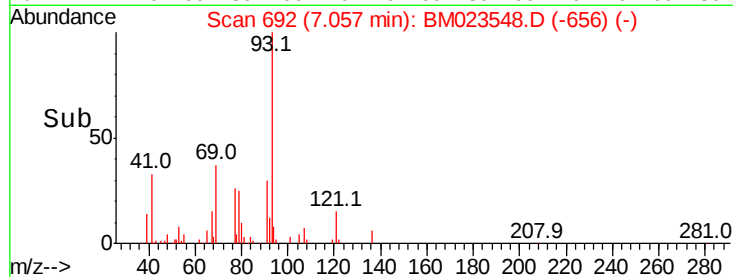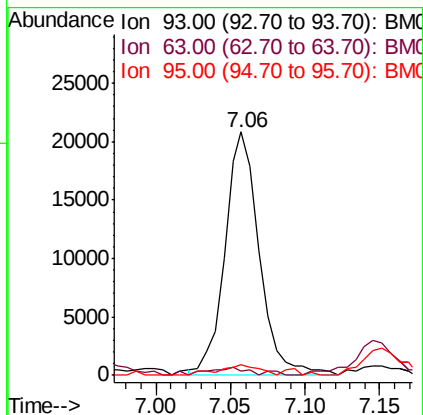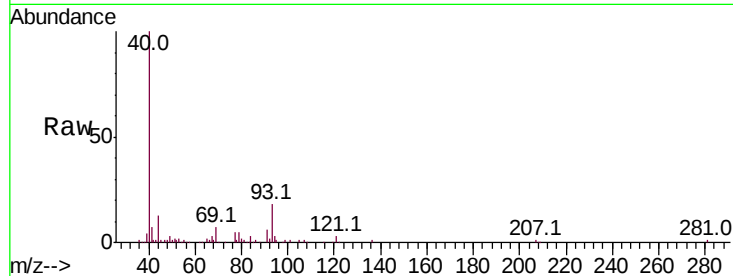

#45

Dimethylphthalate
 Concen: 4.525 ng/ul
 RT: 13.72 min Scan# 1825
 Delta R.T. -0.01 min
 Lab File: BM023548.D
 Acq: 01 Nov 2019 08:15

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.3	4.9
164	10.0	7.9	11.9

