

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
 Data File : BM023529.D
 Acq On : 31 Oct 2019 20:51
 Operator : JU
 Sample : K5426-15
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLNJ5

Quant Time: Nov 01 07:15:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 01 07:12:43 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	400885	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1614958	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	973814	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.01	188	2050436	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	2019533	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	2416419	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	54325	6.44	ng/uL	0.00
5) Phenol-d5	6.79	99	200025	5.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	520275	26.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	578814	21.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	344896	12.61	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	347256	28.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	364968	27.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	626215	23.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	42780	1.40	ng/ul	0.01
44) Dimethylphthalate-d6	13.68	166	2168030	29.32	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2502267	29.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	52963	4.13	ng/ul	0.00
58) Fluorene-d10	15.26	176	1877605	29.98	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	264534	20.72	ng/ul	0.00
71) Anthracene-d10	17.11	188	3172117	32.74	ng/ul	0.00
79) Pyrene-d10	19.41	212	3725510	33.54	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	4467820	36.29	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.72	163	175594	2.365	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
Data File : BM023529.D
Acq On : 31 Oct 2019 20:51
Operator : JU
Sample : K5426-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNJ5

Quant Time: Nov 01 07:15:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 01 07:12:43 2019
Response via : Initial Calibration

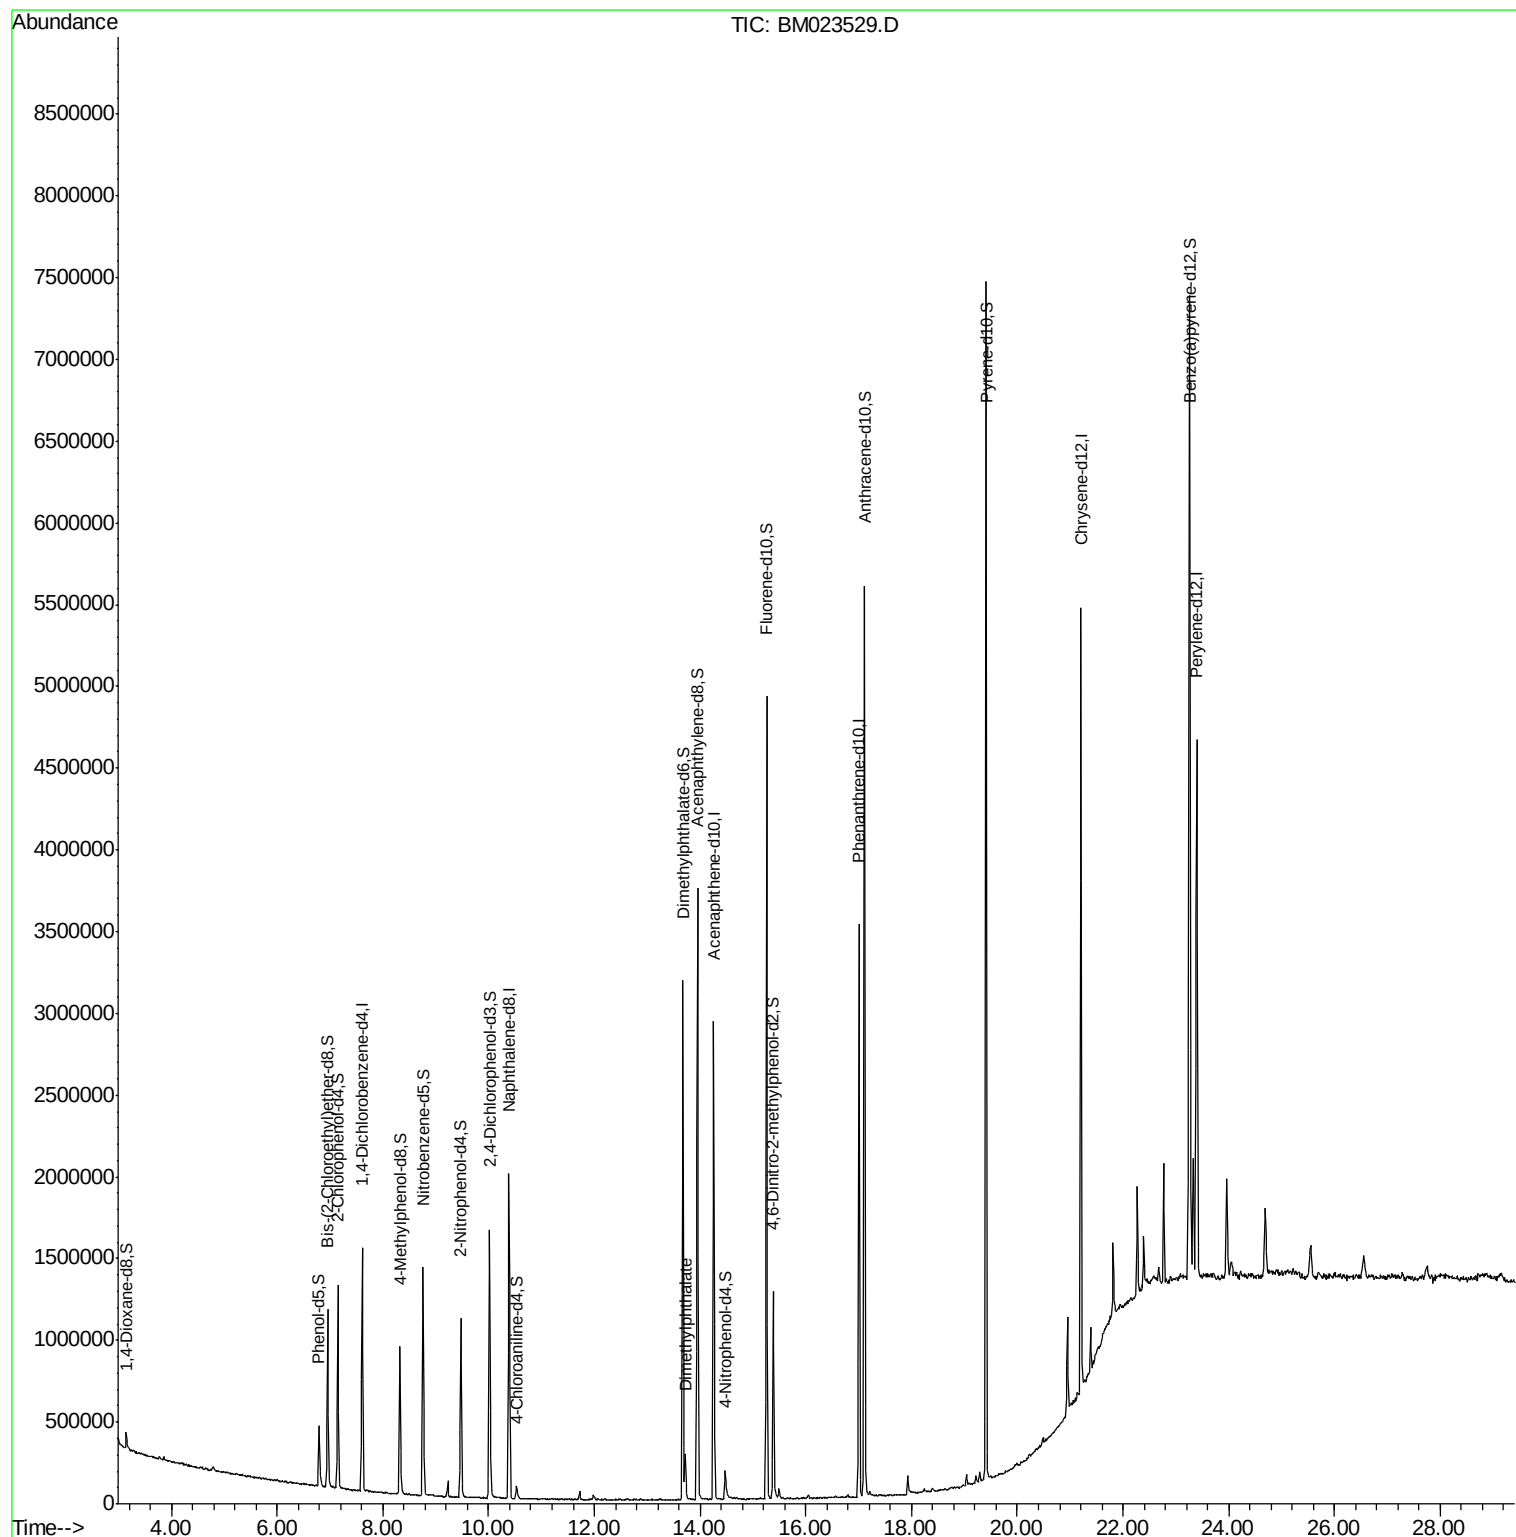

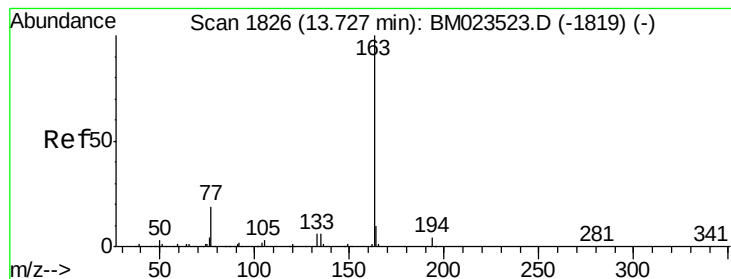

#45

Dimethylphthalate

Concen: 2.365 ng/ul

RT: 13.72 min Scan# 1825

Delta R.T. -0.01 min

Lab File: BM023529.D

Acq: 31 Oct 2019 20:51

Instrument :

BNA_M

ClientSampleId :

JLNJ5


Tot Ion:163 Resp: 175594

Ion Ratio Lower Upper

163 100

194 4.6 3.3 4.9

164 10.2 7.9 11.9

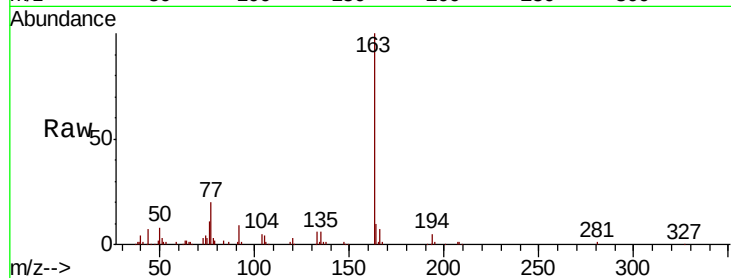

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

