

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
 Data File : BM023535.D
 Acq On : 01 Nov 2019 00:28
 Operator : JU
 Sample : K5433-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLNG2

Quant Time: Nov 01 07:16:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 01 07:12:43 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	369719	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1515086	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	912338	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	1923692	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1911068	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	2282947	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	19465	2.50	ng/uL	0.00
5) Phenol-d5	6.79	99	371552	11.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	242075	13.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	300497	12.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	259142	10.27	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	149476	13.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	151213	11.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	268601	10.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	312883	10.94	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	926065	13.37	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	1051943	13.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	76451	6.37	ng/ul	0.00
58) Fluorene-d10	15.26	176	792246	13.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	75800	6.33	ng/ul	0.00
71) Anthracene-d10	17.10	188	1193329	13.13	ng/ul	0.00
79) Pyrene-d10	19.40	212	1403681	13.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	1606318	13.81	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.82	94	34503	1.079	ng/ul	96
45) Dimethylphthalate	13.72	163	306041	4.400	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
Data File : BM023535.D
Acq On : 01 Nov 2019 00:28
Operator : JU
Sample : K5433-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNG2

Quant Time: Nov 01 07:16:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 01 07:12:43 2019
Response via : Initial Calibration

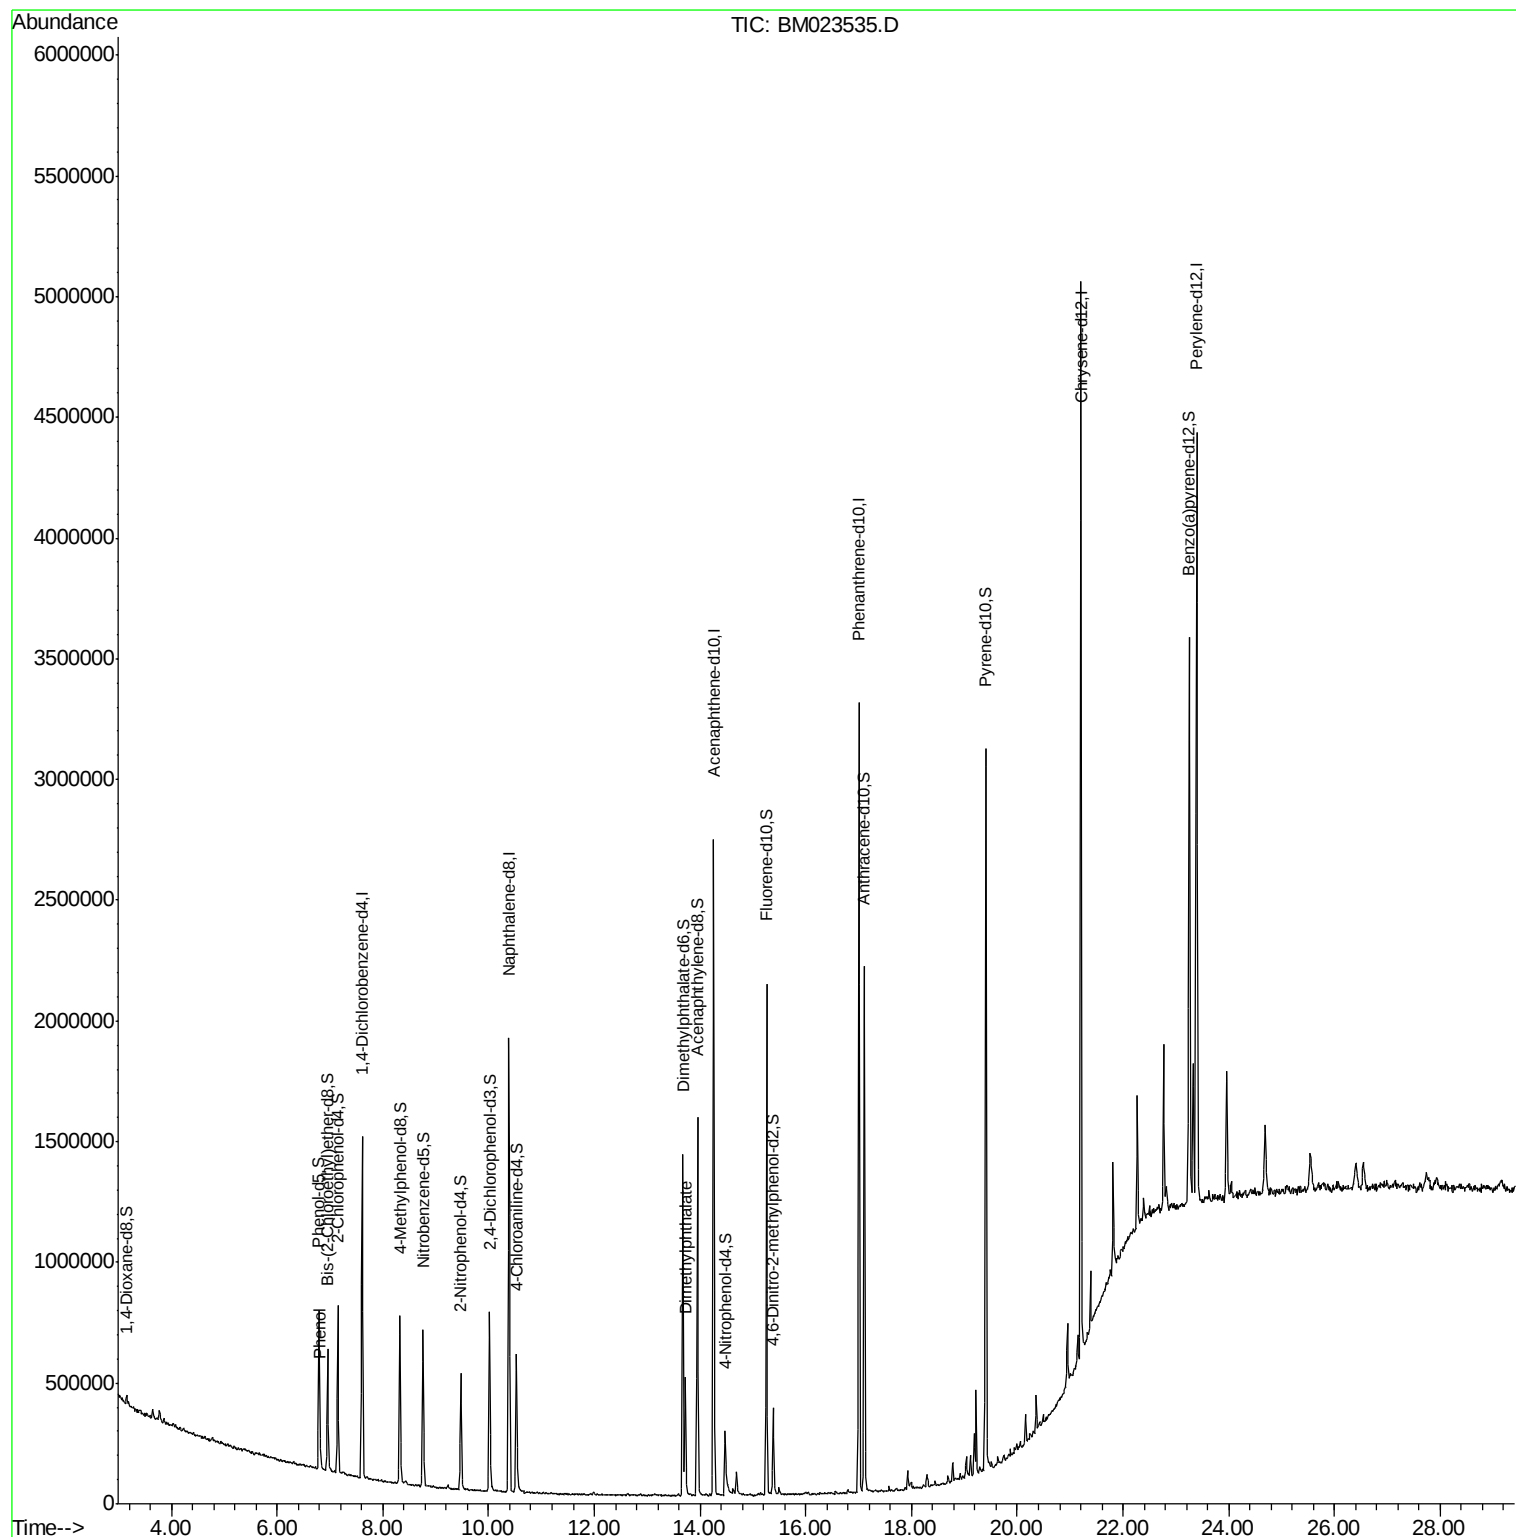

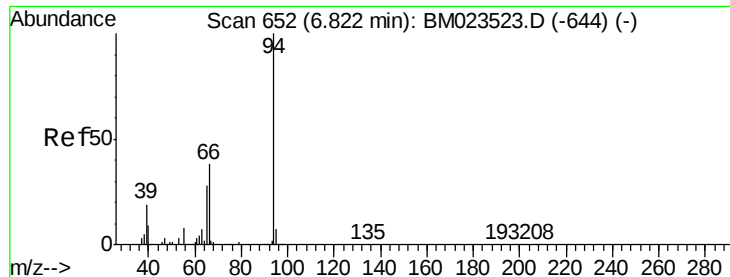





#6

Phenol

Concen: 1.079 ng/ul
 RT: 6.82 min Scan# 651
 Delta R.T. -0.01 min
 Lab File: BM023535.D
 Acq: 01 Nov 2019 00:28

Instrument :
 BNA_M
 ClientSampleId :
 JLNG2

Tot Ion	Ratio	Lower	Upper
94	100		
65	29.6	22.9	34.3
66	42.9	31.4	47.2

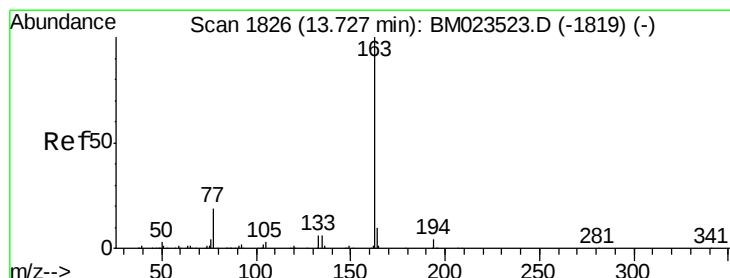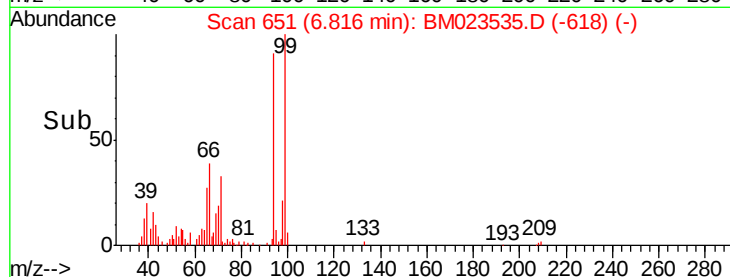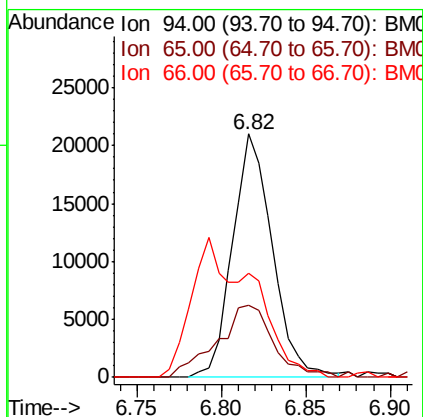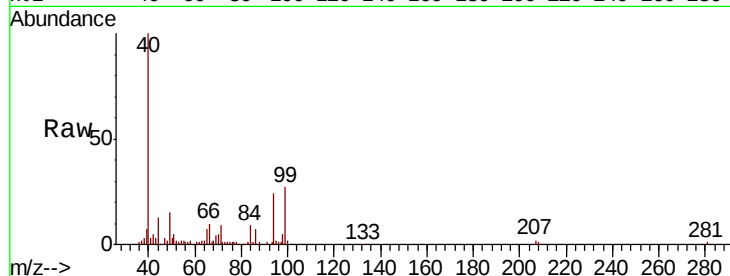

#45

Dimethylphthalate

Concen: 4.400 ng/ul
 RT: 13.72 min Scan# 1825
 Delta R.T. -0.01 min
 Lab File: BM023535.D
 Acq: 01 Nov 2019 00:28

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.3	4.9
164	9.6	7.9	11.9

