

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
 Data File : BM023553.D
 Acq On : 01 Nov 2019 11:22
 Operator : JU
 Sample : K5511-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJL6

Quant Time: Nov 01 13:06:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 01 08:19:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	354810	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1487063	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	904333	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	1910513	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1910804	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	2268591	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	43433	5.81	ng/uL	0.00
5) Phenol-d5	6.79	99	205669	6.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	462752	26.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	525187	22.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	356001	14.71	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	316562	28.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	344865	27.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	613130	25.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	91283	3.25	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	2161627	31.48	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2386304	30.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	66647	5.60	ng/ul	0.00
58) Fluorene-d10	15.26	176	1811392	31.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	252316	21.21	ng/ul	0.00
71) Anthracene-d10	17.10	188	2994903	33.17	ng/ul	0.00
79) Pyrene-d10	19.40	212	3425517	32.60	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	4089664	35.39	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.72	163	292599	4.244	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
Data File : BM023553.D
Acq On : 01 Nov 2019 11:22
Operator : JU
Sample : K5511-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJL6

Quant Time: Nov 01 13:06:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 01 08:19:37 2019
Response via : Initial Calibration

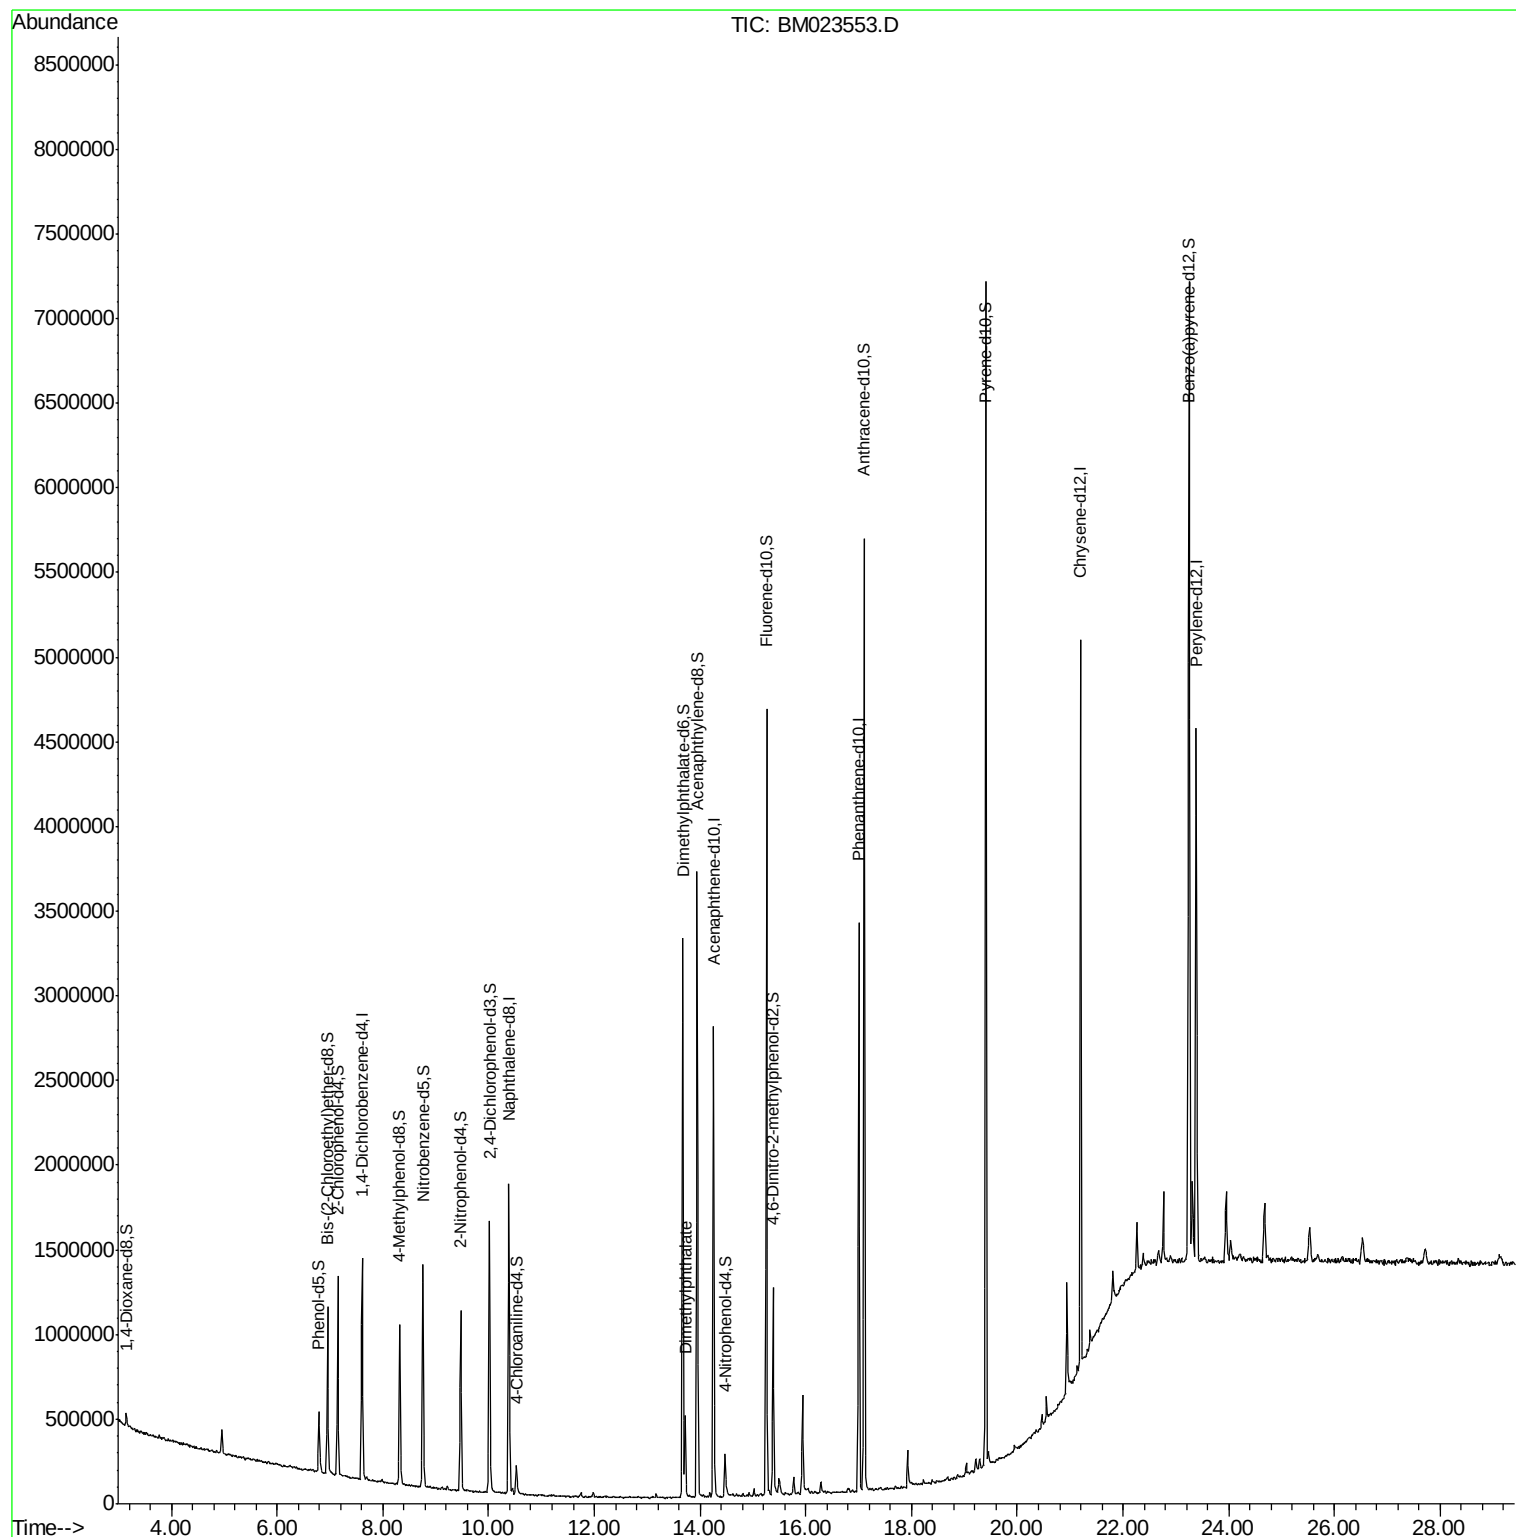

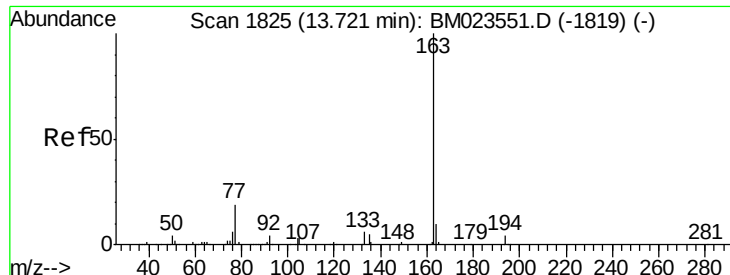

#45

Dimethylphthalate

Concen: 4.244 ng/ul

RT: 13.72 min Scan# 1825

Delta R.T. -0.01 min

Lab File: BM023553.D

Acq: 01 Nov 2019 11:22

Instrument :

BNA_M

ClientSampleId :

BEJL6


Tot Ion:163 Resp: 292599

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 9.8 7.9 11.9

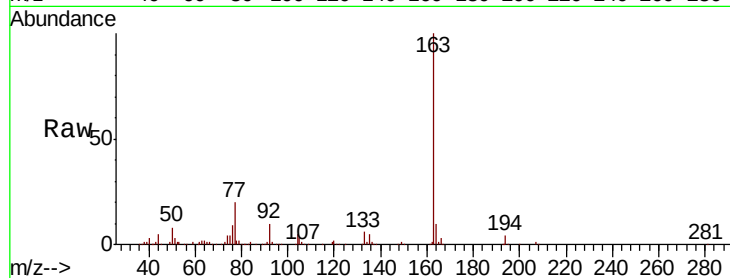

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

