

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
 Data File : BM023561.D
 Acq On : 01 Nov 2019 16:09
 Operator : JU
 Sample : K5511-08
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJM4

Quant Time: Nov 01 16:22:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 01 08:19:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	376439	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1524831	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	918720	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	1919562	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1906385	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	2275308	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	49239	6.21	ng/uL	0.00
5) Phenol-d5	6.79	99	269267	8.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	657904	35.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	728263	29.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	481464	18.75	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	456953	39.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	499294	39.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	819158	32.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	76506	2.66	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	2828625	40.54	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	3290649	41.17	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	78707	6.51	ng/ul	0.00
58) Fluorene-d10	15.25	176	2387810	40.41	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	326113	27.29	ng/ul	0.00
71) Anthracene-d10	17.10	188	3874291	42.71	ng/ul	0.00
79) Pyrene-d10	19.40	212	4260284	40.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	5074319	43.78	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.72	163	89825	1.282	ng/ul#	96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
Data File : BM023561.D
Acq On : 01 Nov 2019 16:09
Operator : JU
Sample : K5511-08
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJM4

Quant Time: Nov 01 16:22:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 01 08:19:37 2019
Response via : Initial Calibration

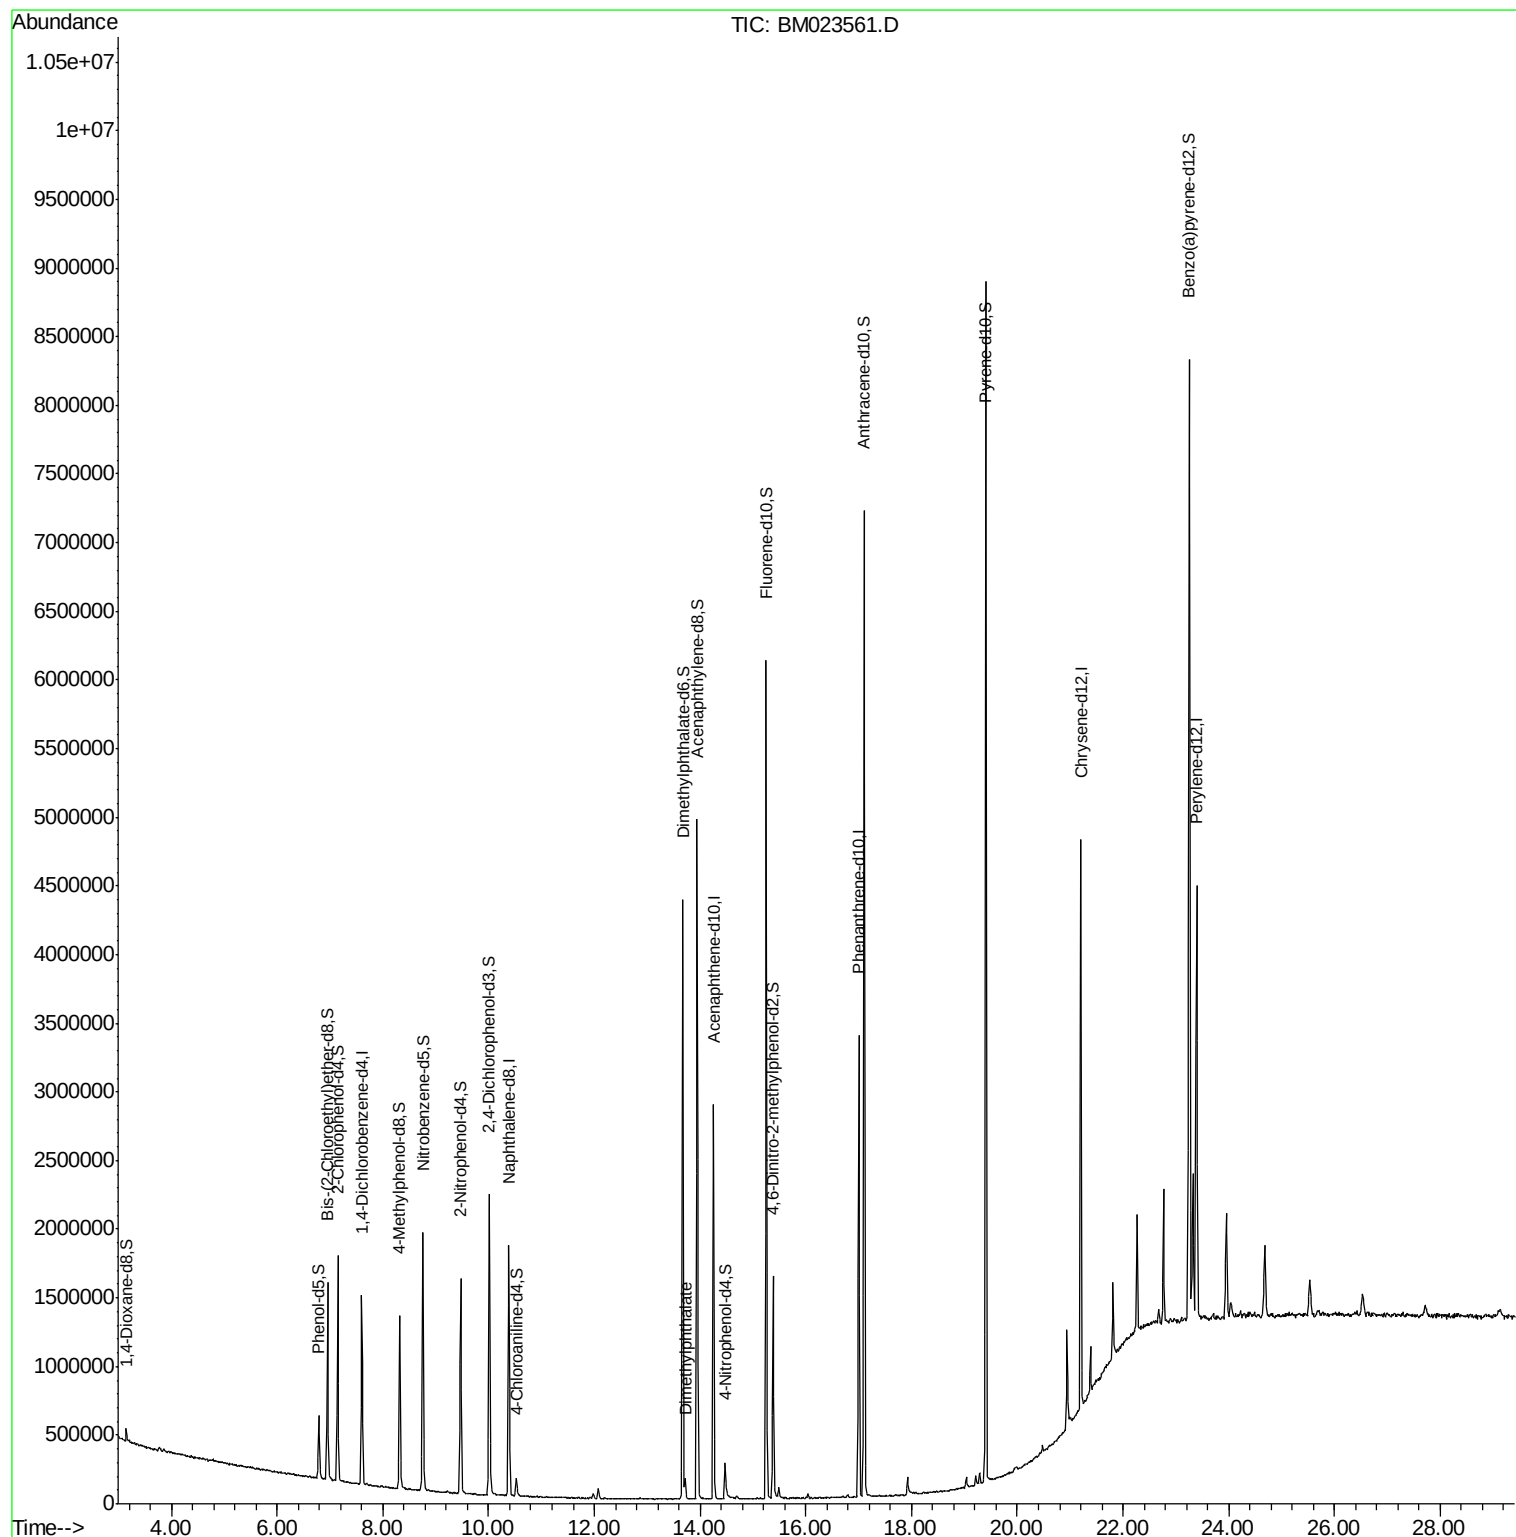

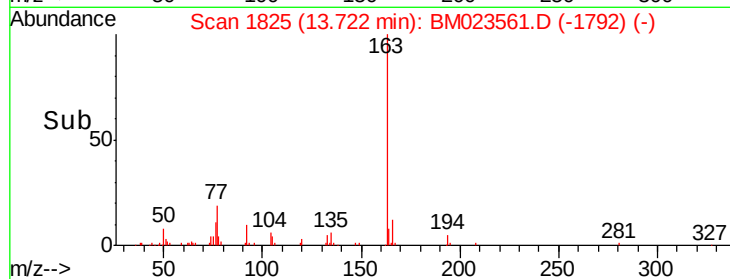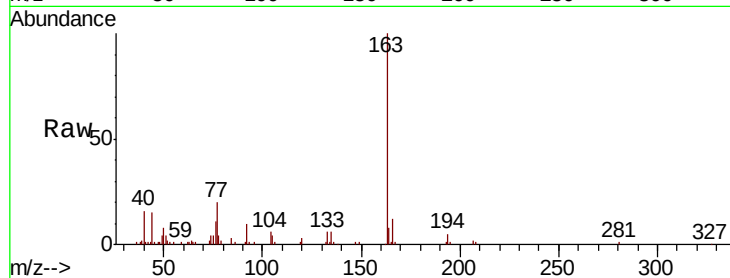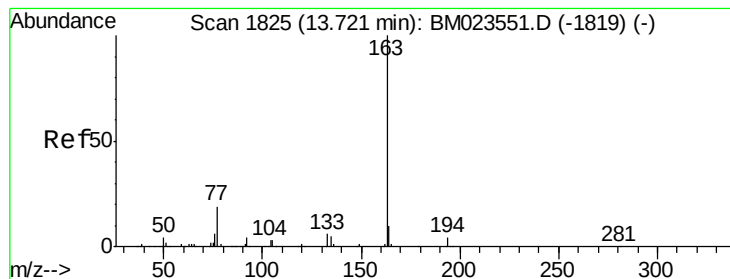

#45

Dimethylphthalate

Concen: 1.282 ng/ul

RT: 13.72 min Scan# 1825

Delta R.T. -0.01 min

Lab File: BM023561.D

Acq: 01 Nov 2019 16:09

Instrument :

BNA_M

ClientSampleId :

BEJM4

Tot Ion:163 Resp: 89825

Ion Ratio Lower Upper

163 100

194 5.0 3.3 4.9#

164 8.4 7.9 11.9

