

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
 Data File : BM023563.D
 Acq On : 01 Nov 2019 17:21
 Operator : JU
 Sample : K5511-10
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJM6

Quant Time: Nov 01 16:53:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 01 08:19:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	405953	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	1644500	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	984349	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	2036012	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1955140	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	2354125	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	58775	6.88	ng/uL	0.00
5) Phenol-d5	6.79	99	302535	8.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	624914	31.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	713889	26.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	503660	18.19	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	418722	33.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	450719	32.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	767888	28.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	85059	2.74	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	2682199	35.88	ng/ul	0.00
47) Acenaphthylene-d8	13.94	160	3066124	35.81	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	84847	6.55	ng/ul	0.00
58) Fluorene-d10	15.25	176	2261909	35.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	312307	24.64	ng/ul	0.00
71) Anthracene-d10	17.10	188	3701826	38.47	ng/ul	0.00
79) Pyrene-d10	19.40	212	4018885	37.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	4801633	40.04	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.72	163	87175	1.162	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
Data File : BM023563.D
Acq On : 01 Nov 2019 17:21
Operator : JU
Sample : K5511-10
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJM6

Quant Time: Nov 01 16:53:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 01 08:19:37 2019
Response via : Initial Calibration

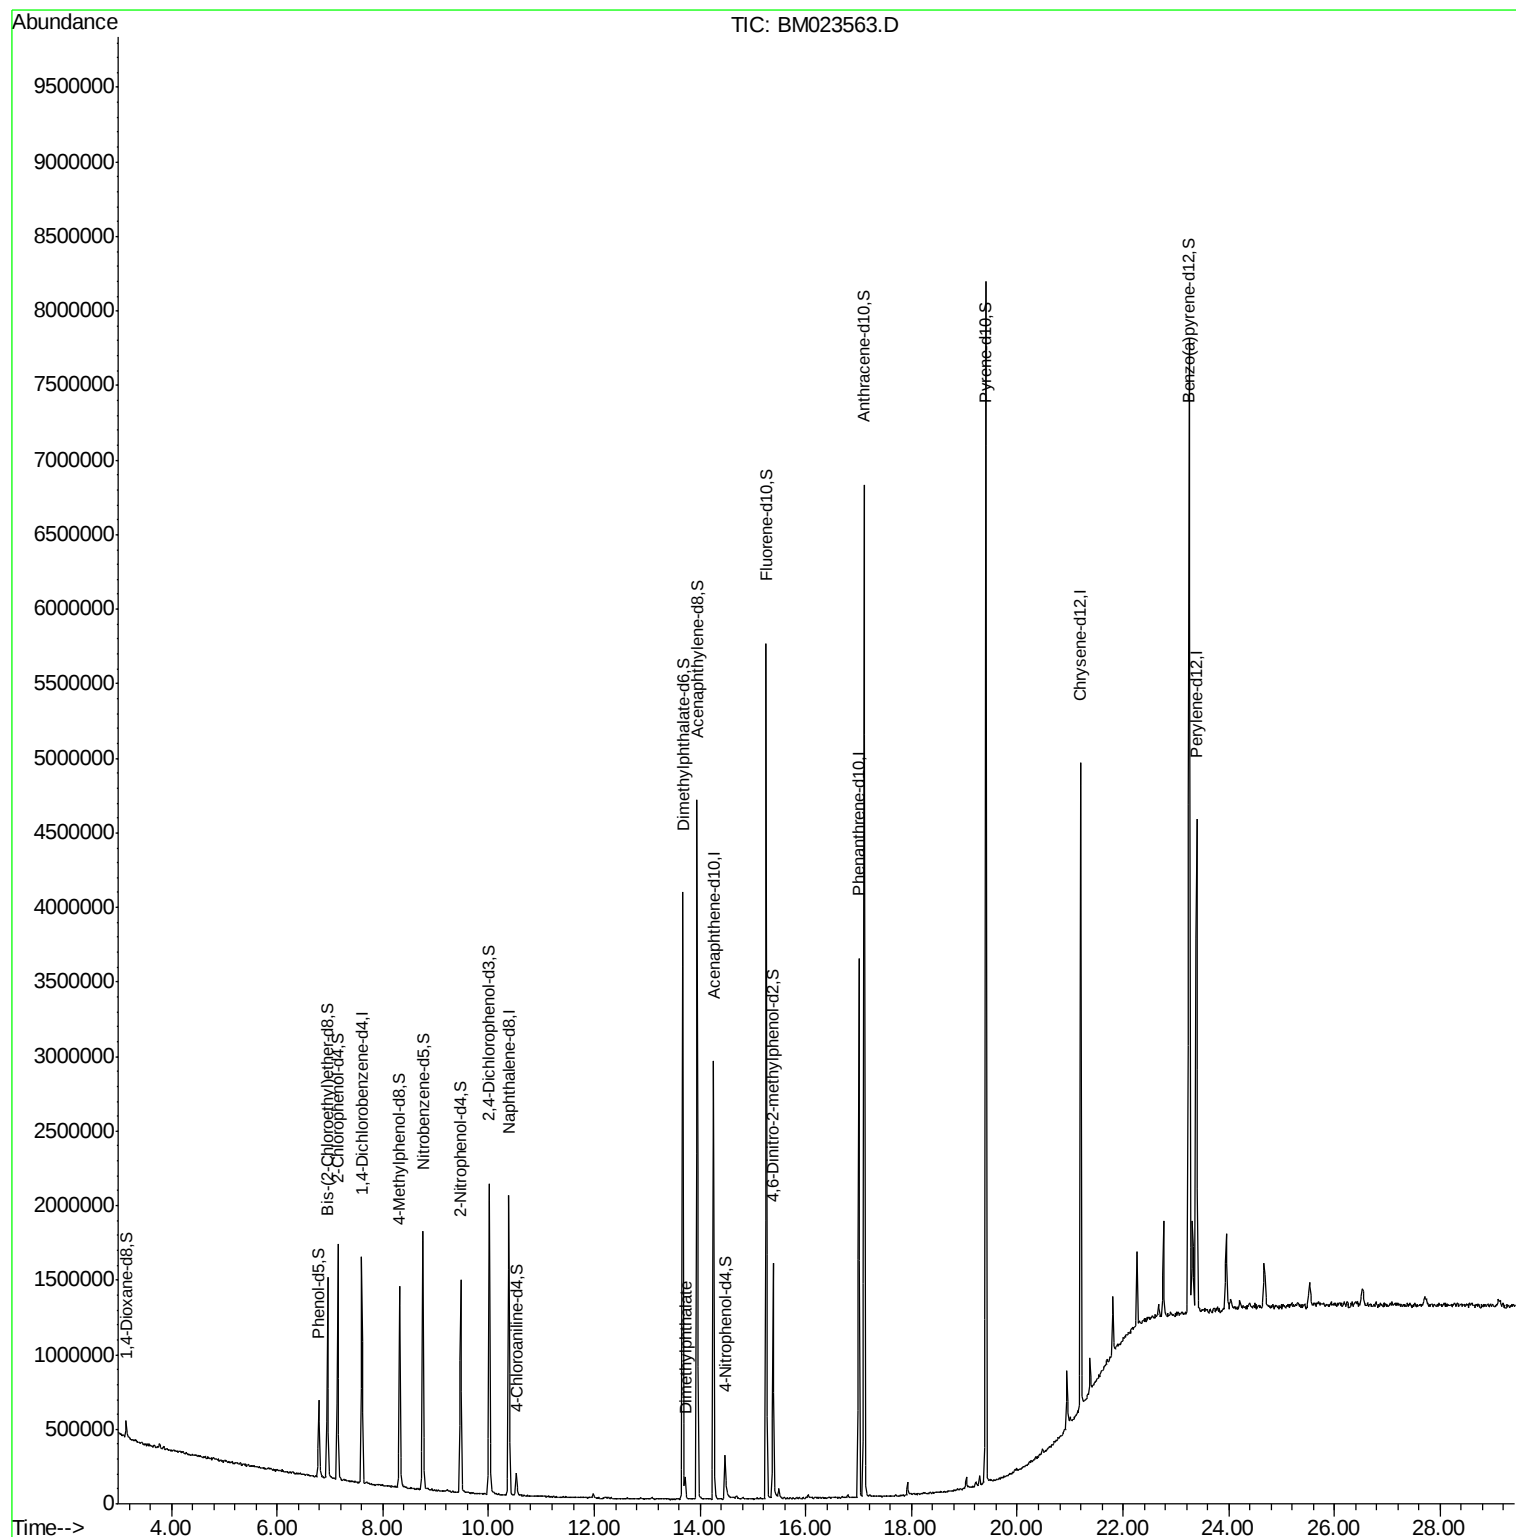

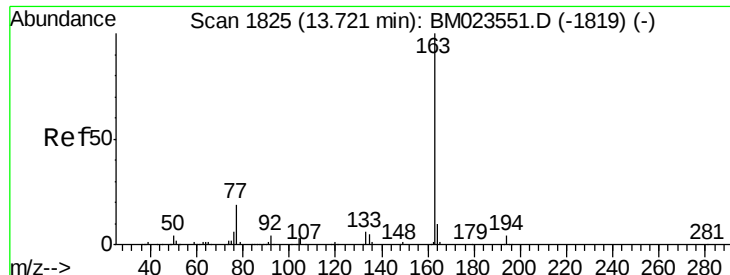

#45

Dimethylphthalate

Concen: 1.162 ng/ul

RT: 13.72 min Scan# 1825

Delta R.T. -0.01 min

Lab File: BM023563.D

Acq: 01 Nov 2019 17:21

Instrument :

BNA_M

ClientSampleId :

BEJM6


Tot Ion:163 Resp: 87175

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.5 7.9 11.9

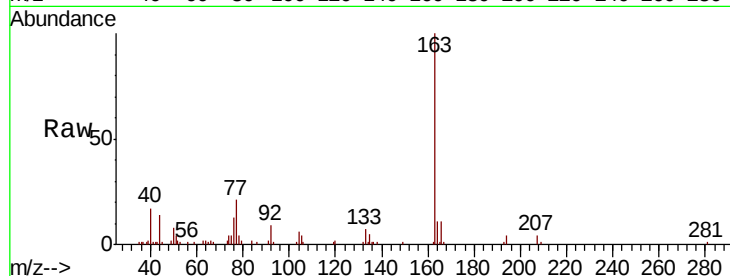

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

