

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
 Data File : BM023567.D
 Acq On : 01 Nov 2019 20:20
 Operator : JU
 Sample : K5511-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJM7

Quant Time: Nov 04 01:10:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 04 01:07:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	435960	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	1783295	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	1068373	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	2222907	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	2133146	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	2549916	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	57577	6.27	ng/uL	0.00
5) Phenol-d5	6.79	99	271079	7.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	688379	32.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	740366	25.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	493299	16.59	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	467456	34.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	504909	33.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	838339	28.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	84254	2.50	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	2906996	35.83	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	3394681	36.52	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	74897	5.33	ng/ul	0.00
58) Fluorene-d10	15.25	176	2454067	35.72	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	327644	23.67	ng/ul	0.00
71) Anthracene-d10	17.10	188	3824792	36.41	ng/ul	0.00
79) Pyrene-d10	19.40	212	4169402	35.54	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	4916204	37.85	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.72	163	142387	1.748 ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
Data File : BM023567.D
Acq On : 01 Nov 2019 20:20
Operator : JU
Sample : K5511-11
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJM7

Quant Time: Nov 04 01:10:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 04 01:07:42 2019
Response via : Initial Calibration

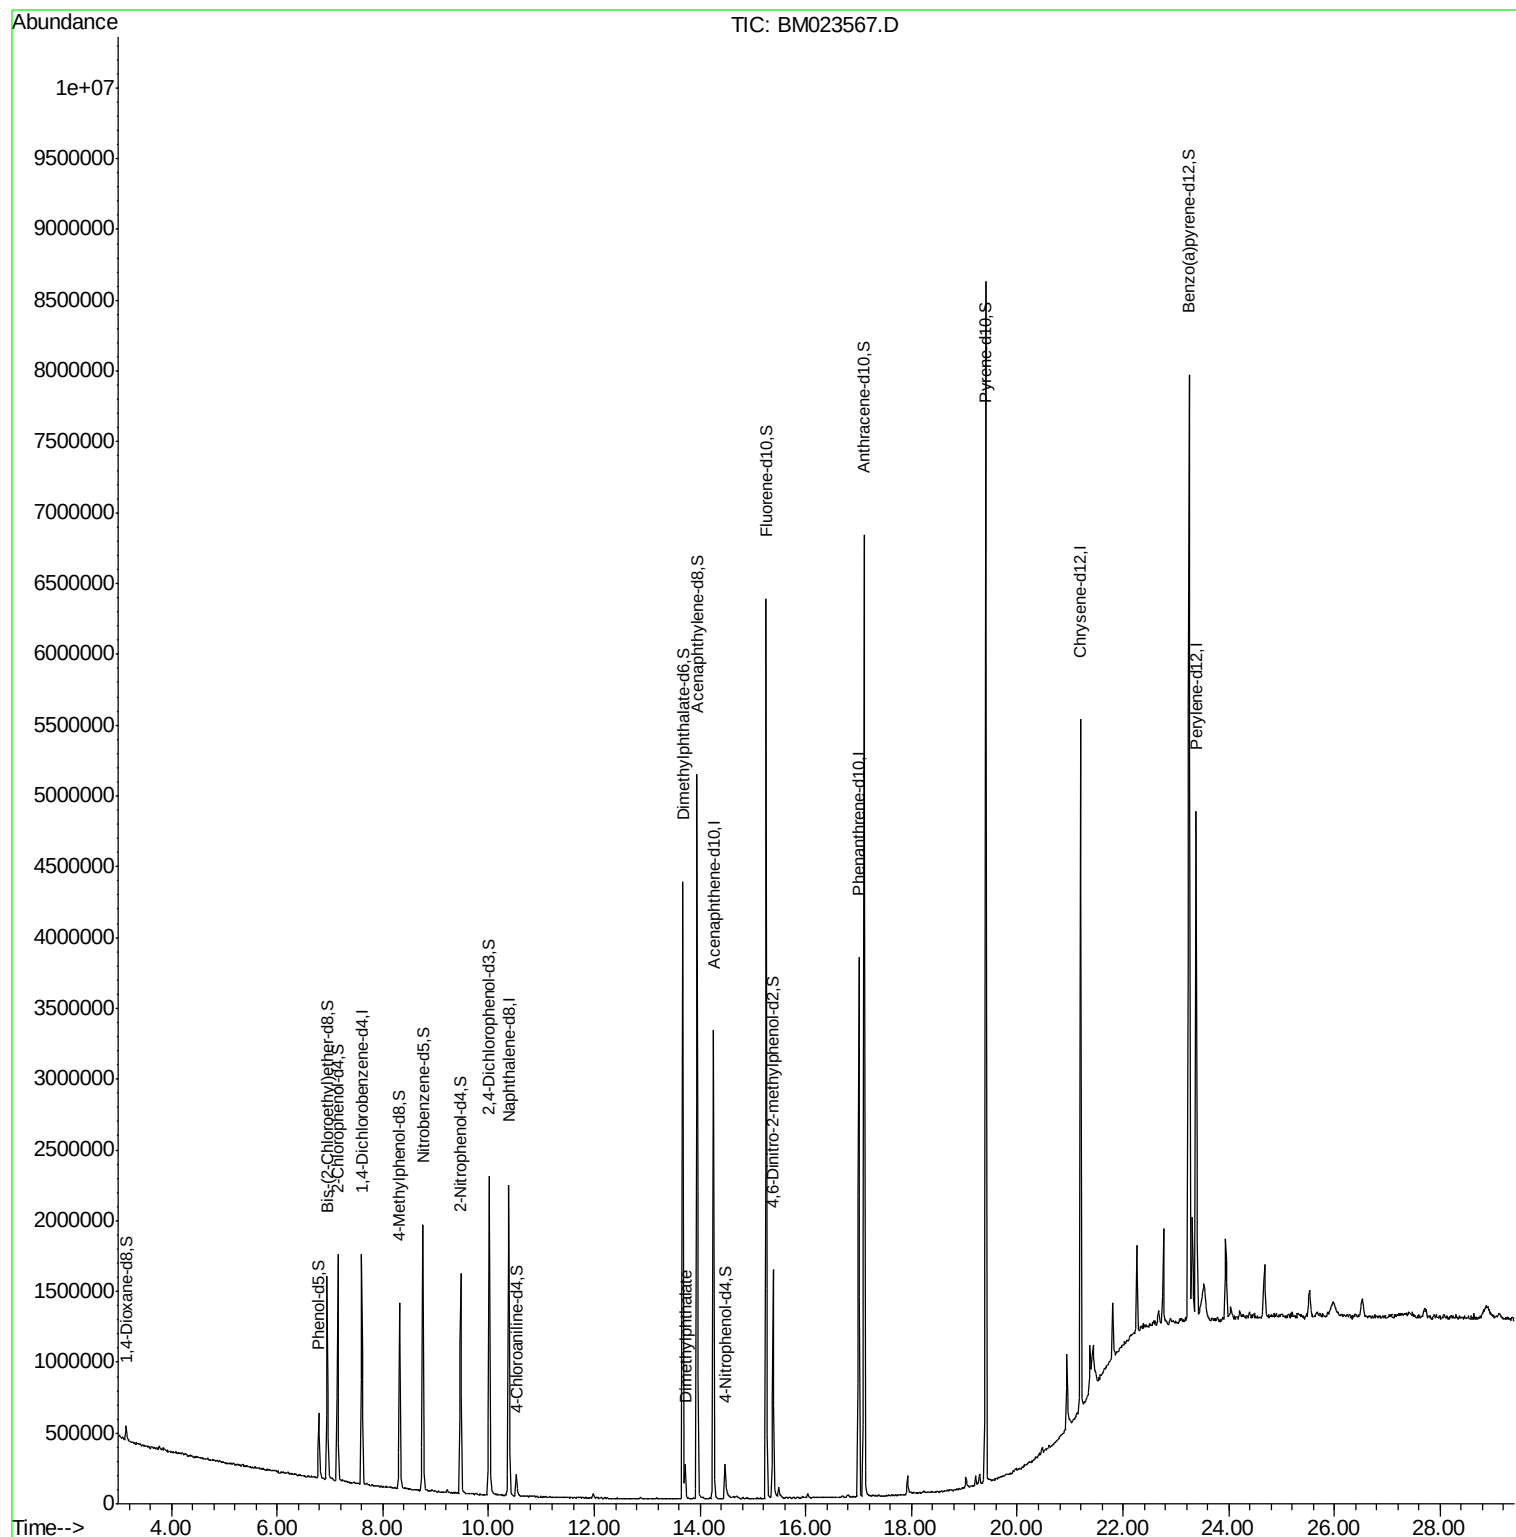

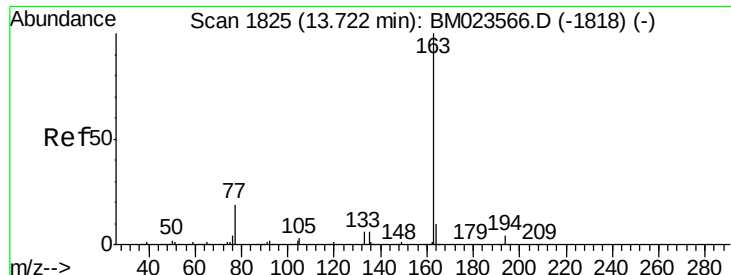

#45

Dimethylphthalate

Concen: 1.748 ng/ul

RT: 13.72 min Scan# 1825

Delta R.T. 0.00 min

Lab File: BM023567.D

Acq: 01 Nov 2019 20:20

Instrument :

BNA_M

ClientSampleId :

BEJM7


Tot Ion:163 Resp: 142387

Ion Ratio Lower Upper

163 100

194 3.9 3.3 4.9

164 9.3 7.9 11.9

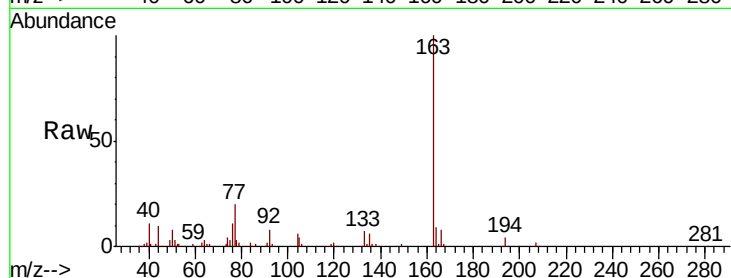

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

