

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
 Data File : BM023565.D
 Acq On : 01 Nov 2019 18:32
 Operator : JU
 Sample : PB124285BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.787	641	646	658	rVB	497074	810887	6.38%	0.733%
2	6.951	668	674	682	rBV	1433533	2338277	18.38%	2.113%
3	7.145	701	707	715	rVB	1634747	2640782	20.76%	2.386%
4	7.604	779	785	795	rVB	1527242	2389651	18.79%	2.159%
5	8.316	900	906	914	rBV	1363665	2176656	17.11%	1.967%
6	8.428	922	925	931	rVB	48170	75595	0.59%	0.068%
7	8.757	974	981	996	rVB	1948663	3245492	25.52%	2.932%
8	8.898	1000	1005	1010	rBV3	20475	39911	0.31%	0.036%
9	9.475	1096	1103	1112	rBV	1588705	2634887	20.72%	2.381%
10	10.010	1187	1194	1207	rBV	2273743	3835720	30.16%	3.466%
11	10.381	1250	1257	1268	rVB	2072596	3472348	27.30%	3.137%
12	11.986	1523	1530	1534	rBV3	37766	65531	0.52%	0.059%
13	13.674	1810	1817	1829	rBV	4775796	6577019	51.71%	5.943%
14	13.945	1855	1863	1875	rBV	5259553	7613167	59.86%	6.879%
15	14.257	1907	1916	1926	rBV	3103960	4607296	36.22%	4.163%
16	14.474	1945	1953	1975	rBV	300565	677464	5.33%	0.612%
17	15.086	2054	2057	2063	rVB7	8803	17322	0.14%	0.016%
18	15.251	2079	2085	2097	rBV	6956865	9770169	76.82%	8.828%
19	15.380	2100	2107	2117	rBV	1785314	2491759	19.59%	2.251%
20	15.492	2121	2126	2132	rVB2	76164	121304	0.95%	0.110%
21	16.039	2215	2219	2223	rBV3	27686	37125	0.29%	0.034%
22	16.686	2325	2329	2335	rVB8	11563	18117	0.14%	0.016%
23	16.792	2342	2347	2354	rBV3	17443	30772	0.24%	0.028%
24	17.004	2376	2383	2390	rBV	3730084	5200415	40.89%	4.699%
25	17.104	2393	2400	2412	rVV	7427274	10528942	82.78%	9.513%
26	17.921	2533	2539	2542	rBV7	30017	48350	0.38%	0.044%
27	19.033	2725	2728	2735	rVB	80761	103071	0.81%	0.093%
28	19.203	2755	2757	2763	rBV6	14289	20838	0.16%	0.019%
29	19.286	2767	2771	2776	rVV2	64142	95284	0.75%	0.086%
30	19.403	2785	2791	2807	rBV	9376472	12152302	95.54%	10.980%
31	20.892	3040	3044	3048	rVB	140841	208377	1.64%	0.188%
32	20.945	3049	3053	3057	rVV	352660	413962	3.25%	0.374%
33	20.992	3057	3061	3068	rVV	808415	971247	7.64%	0.878%
34	21.197	3091	3096	3107	rBV	4595253	6011213	47.26%	5.431%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
Data File : BM023565.D
Acq On : 01 Nov 2019 18:32
Operator : JU
Sample : PB124285BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK85

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Title : SVOA CALIBRATION

35	21.380	3125	3127	3131	rBV2	132334	132381	1.04%	0.120%
36	23.250	3439	3445	3453	rBV	7071065	12719087	100.00%	11.492%
37	23.391	3463	3469	3483	rVB	3483663	6383715	50.19%	5.768%


Sum of corrected areas: 110676435

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
Data File : BM023565.D
Acq On : 01 Nov 2019 18:32
Operator : JU
Sample : PB124285BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK85

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

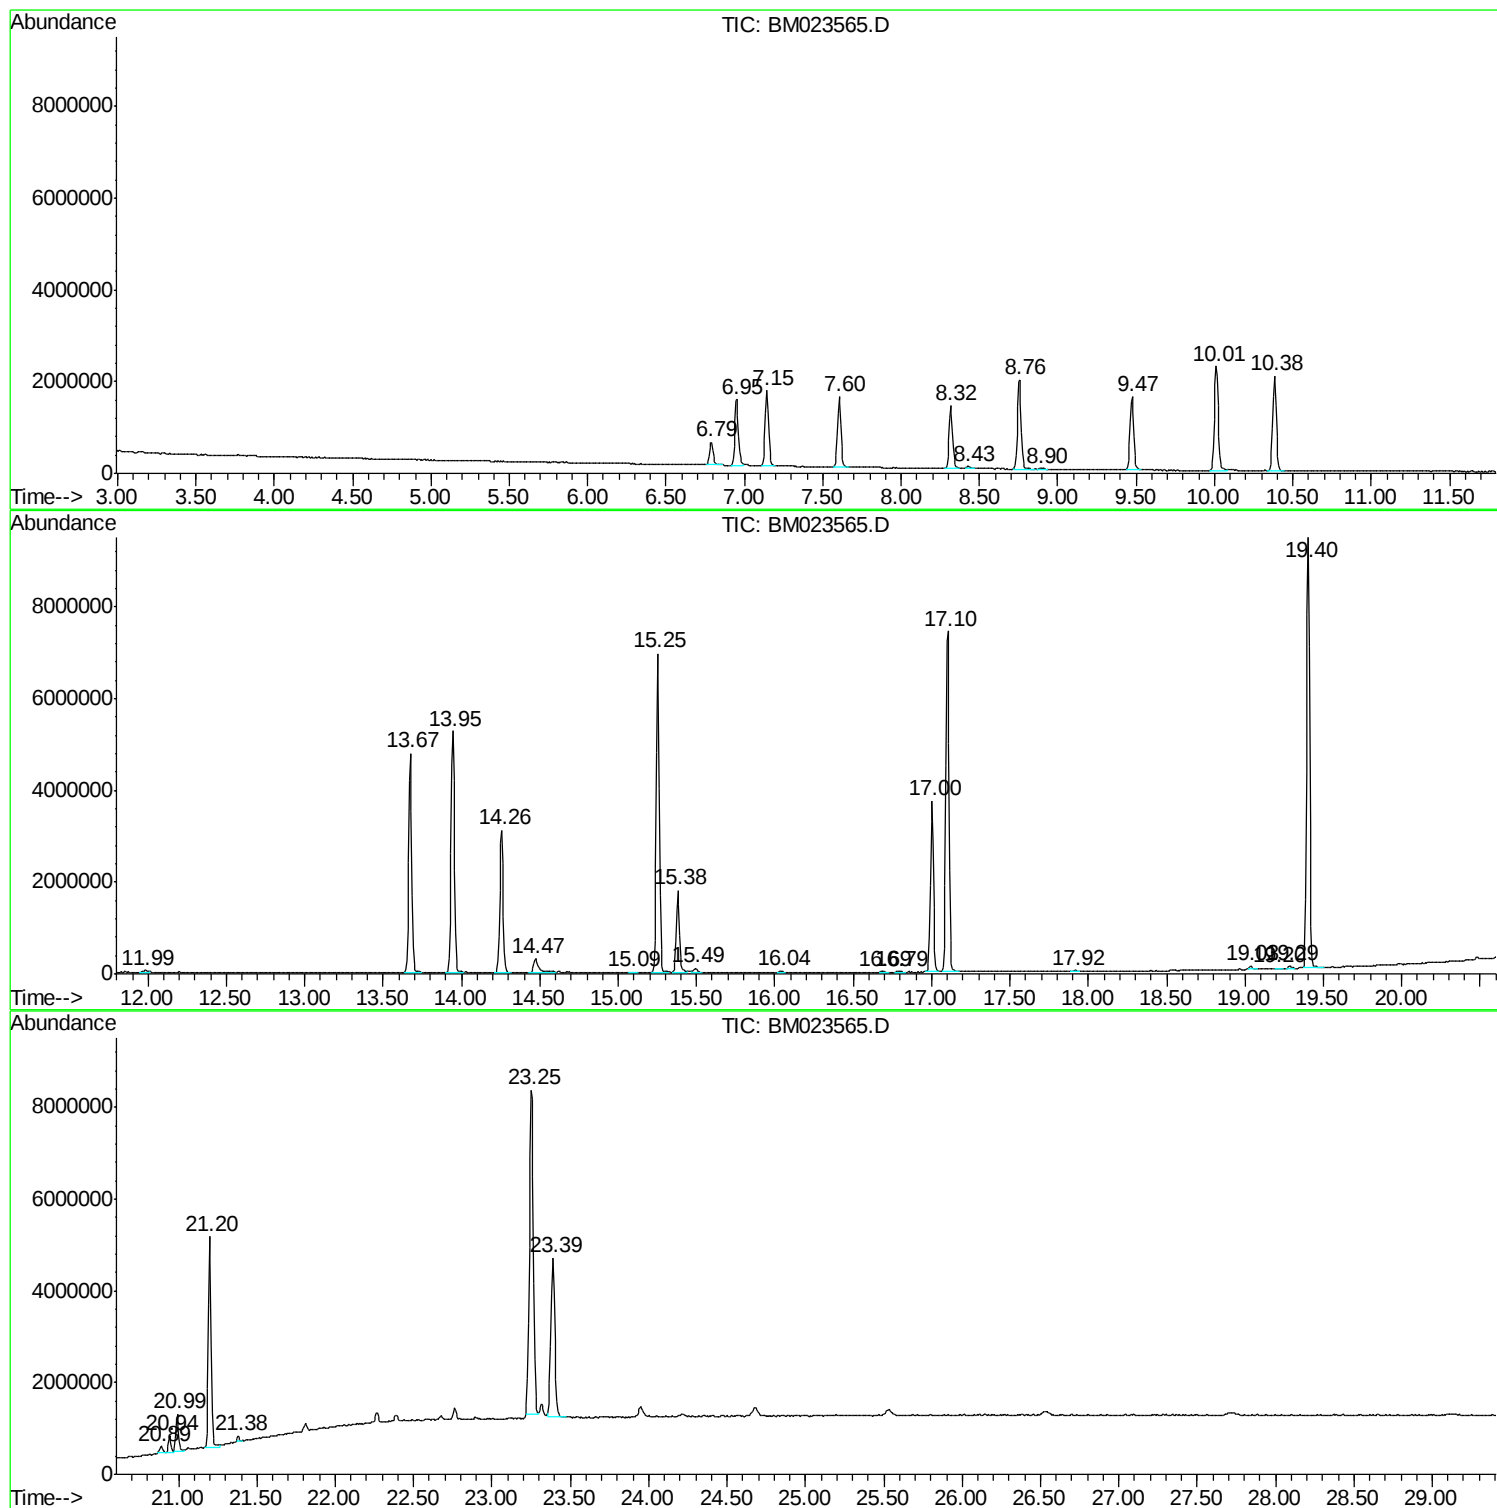

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM103119\
Data File : BM023565.D
Acq On : 01 Nov 2019 18:32
Operator : JU
Sample : PB124285BL
Misc :
ALS Vial : 43 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
SBLK85

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethylene glycol dibenzoate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
20.99	3.23 ng/ul	971247	Chrysene-d12		21.20	
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	64
2		2-(2-Carboxyvinyl)pyridine, trans	149	C8H7NO2	007340-22-9	52
3		2-Methyl-4-hydroxybenzoxazole	149	C8H7NO2	051110-60-2	43
4		Thiophene-2-carboxaldehyde, 3-be...	248	C12H8O2S2	016237-89-1	38
5		Benzamide, N-(3,4-dihydro-2-cyan...	328	C22H20N2O	136819-71-1	35

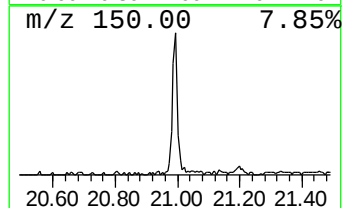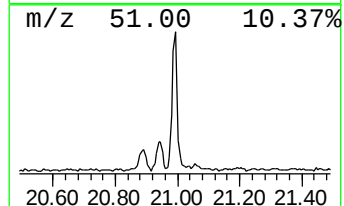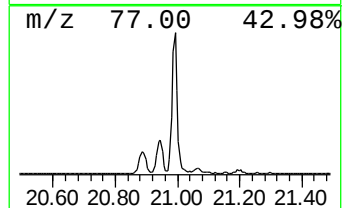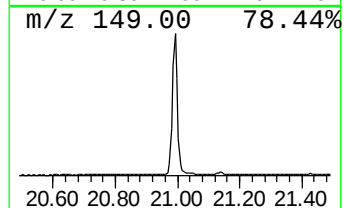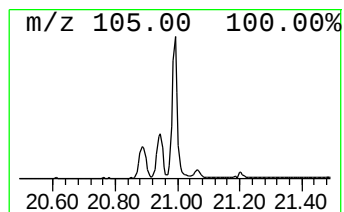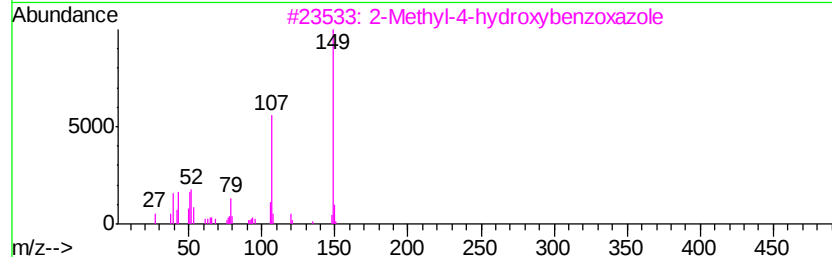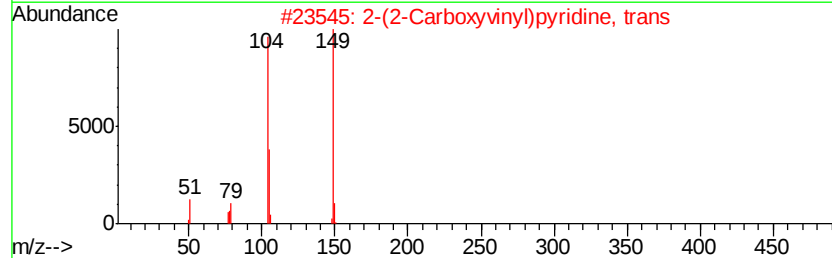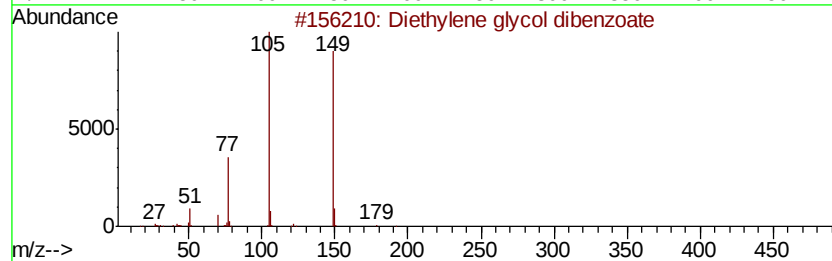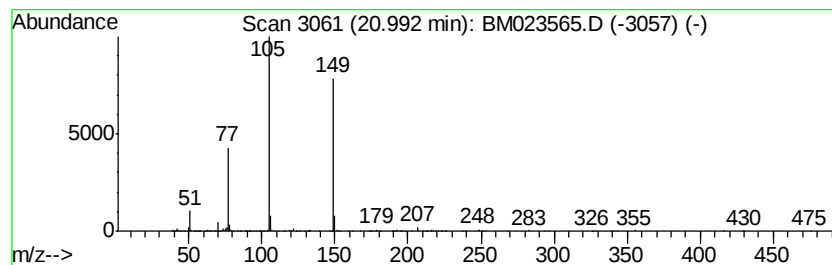

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM103119\
Data File : BM023565.D
Acq On : 01 Nov 2019 18:32
Operator : JU
Sample : PB124285BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK85

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethylene glycol...	20.99	3.2	ng/ul	971247	5	21.20	6011210	20.0