
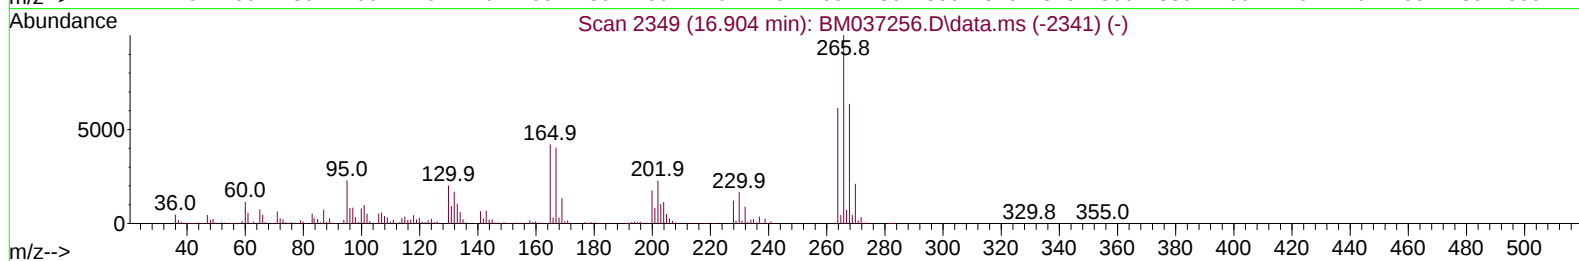
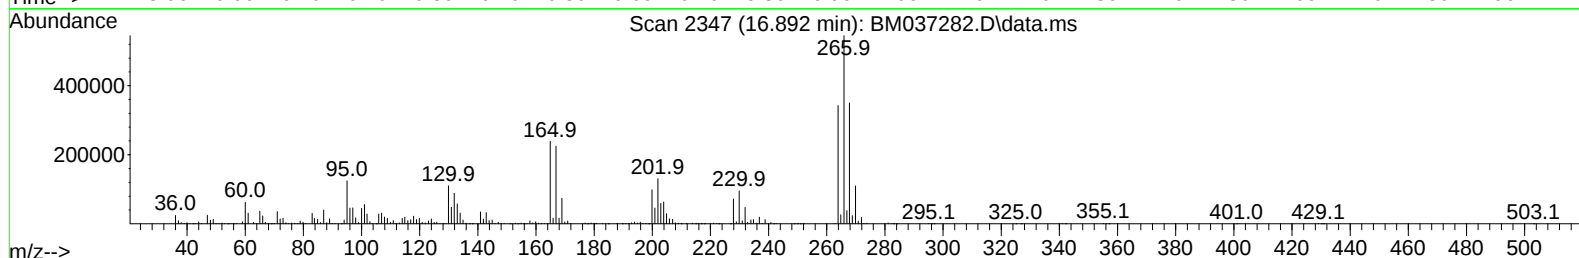


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103122\
Data File : BM037282.D
Acq On : 31 Oct 2022 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 06:23:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 31 01:34:15 2022
Response via : Initial Calibration

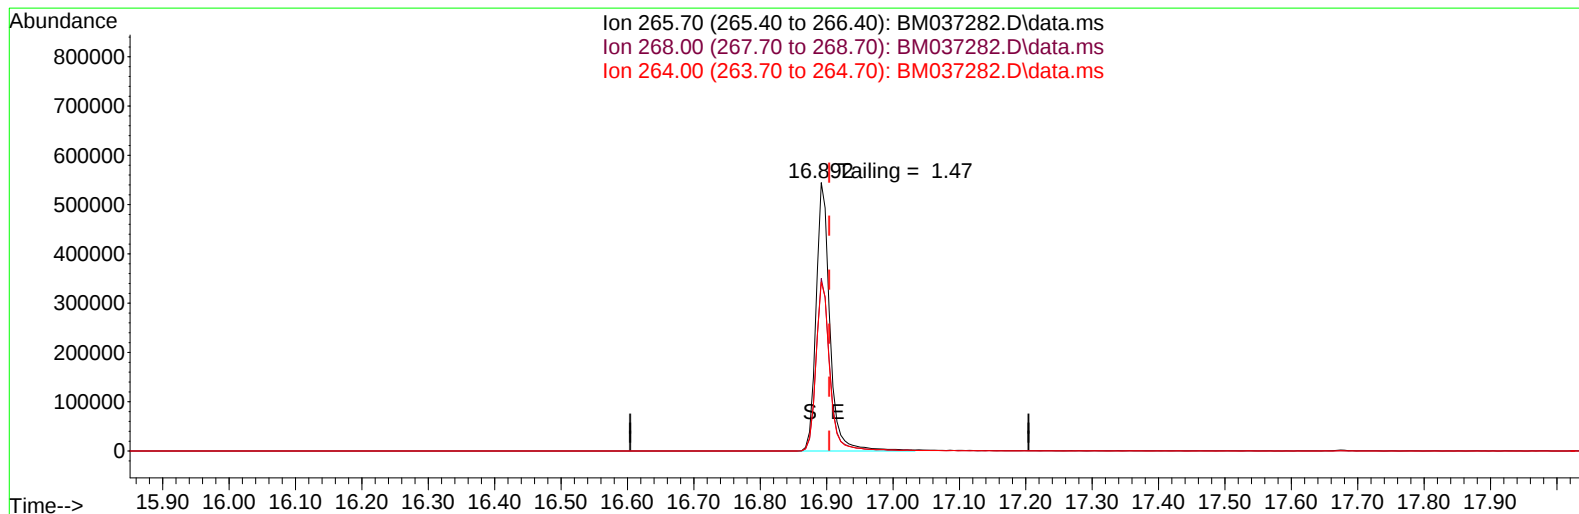

TIC: BM037282.D\data.ms

(70) Pentachlorophenol (C)




16.892min (-0.012) 1812613.78 ng

response 787819

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	64.28
264.00	61.40	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103122\
Data File : BM037282.D
Acq On : 31 Oct 2022 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 06:23:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 31 01:34:15 2022
Response via : Initial Calibration

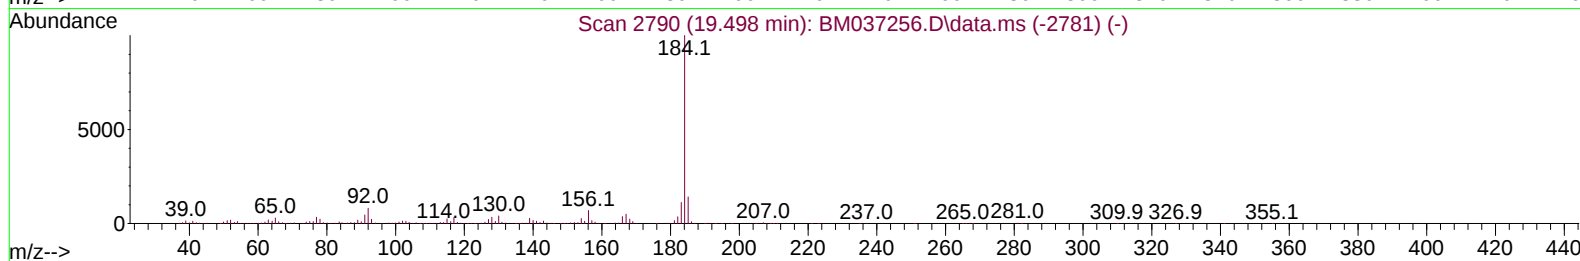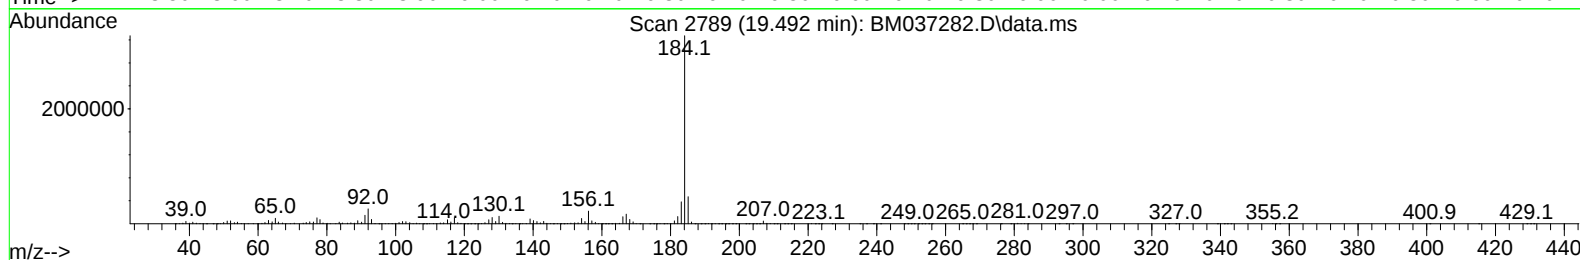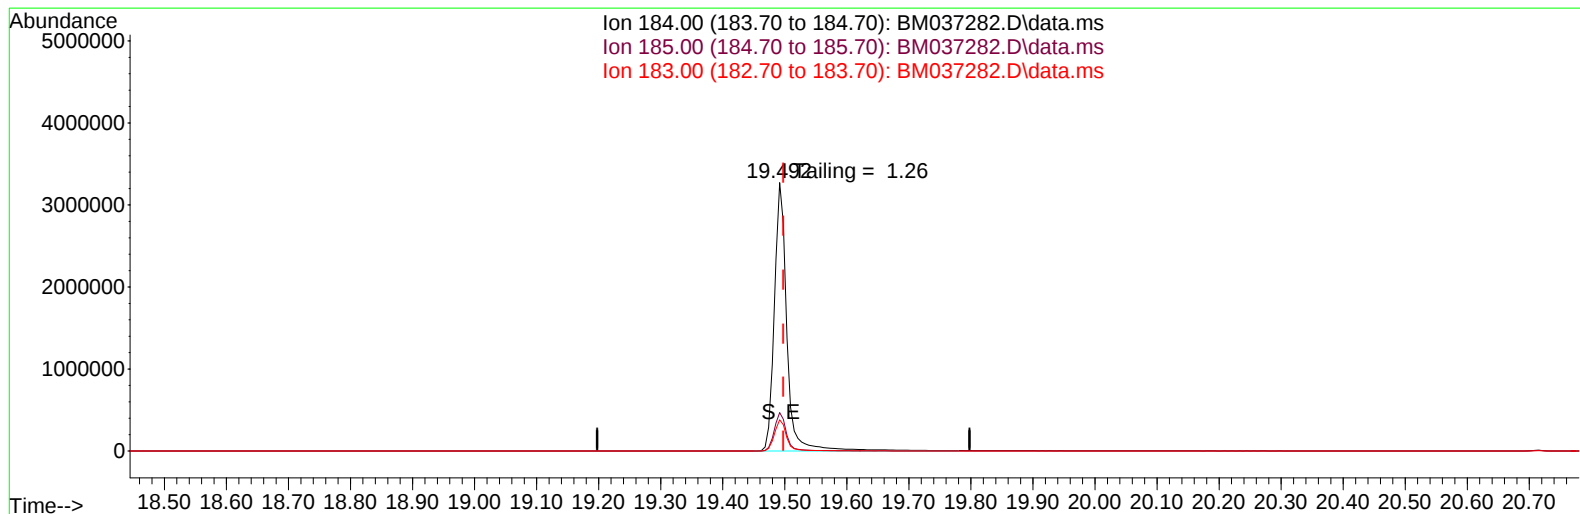

TIC: BM037282.D\data.ms

(77) Benzidine**19.492min (-0.006) 344897.83 ng****response 4628614**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.35
183.00	11.20	11.64
0.00	0.00	0.00