
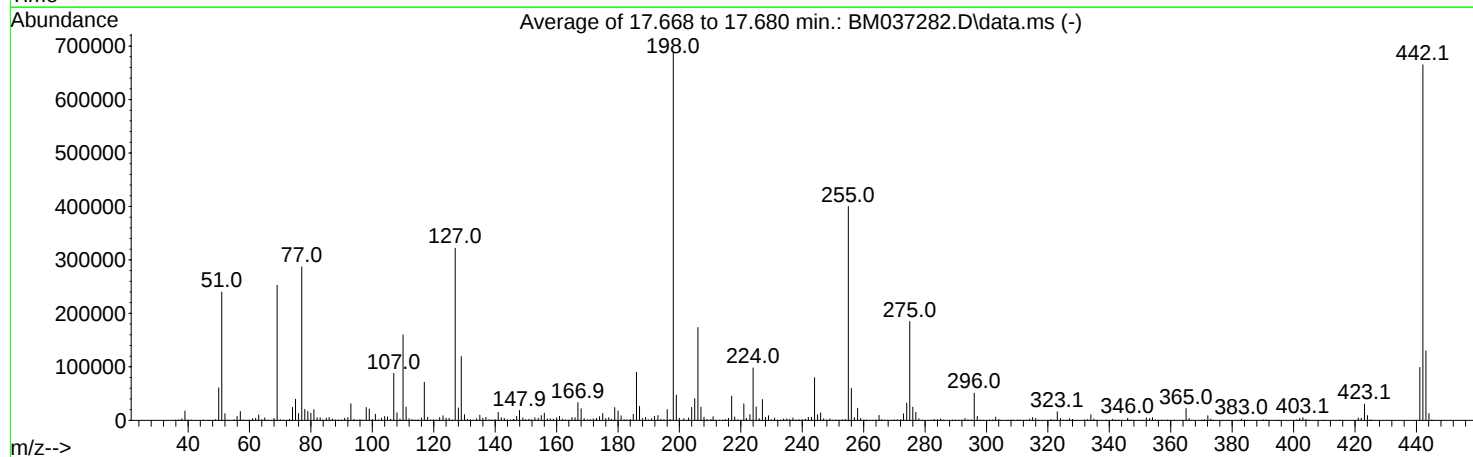


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103122\
 Data File : BM037282.D
 Acq On : 31 Oct 2022 09:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 31 01:34:15 2022

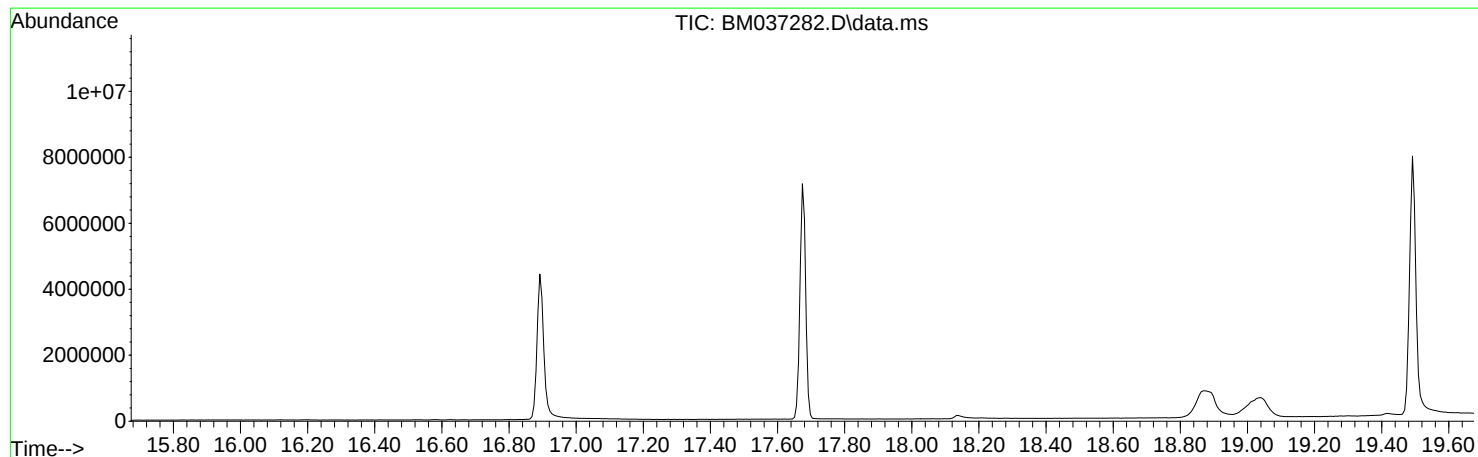




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	239866	PASS
68	69	0.00	2	1.4	3633	PASS
69	198	0.00	100	36.7	252327	PASS
70	69	0.00	2	0.6	1388	PASS
127	198	10	80	46.8	321792	PASS
197	198	0.00	2	0.3	1721	PASS
198	198	100	100	100.0	688085	PASS
199	198	5	9	6.8	47048	PASS
275	198	10	60	26.9	184960	PASS
365	198	1	100	3.2	21977	PASS
441	198	0.01	100	14.4	99032	PASS
442	442	50	100	100.0	664811	PASS
443	442	15	24	19.5	129624	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103122\
Data File : BM037282.D
Acq On : 31 Oct 2022 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 01 06:23:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 31 01:34:15 2022
Response via : Initial Calibration

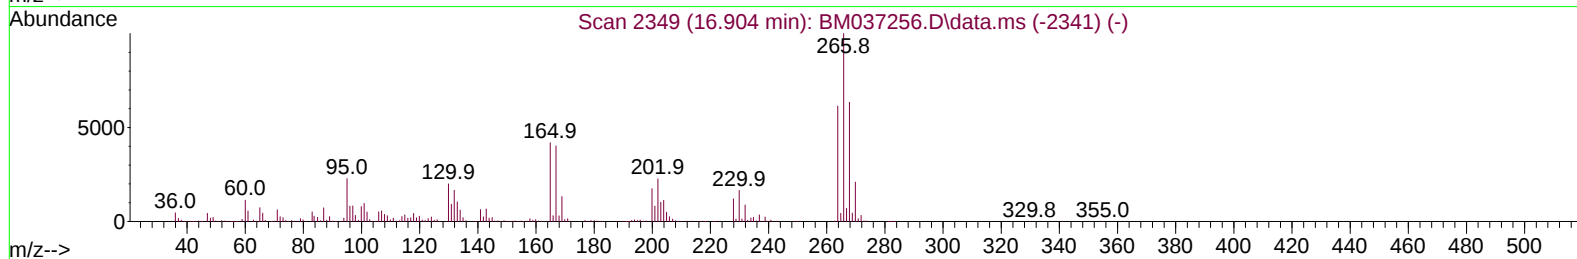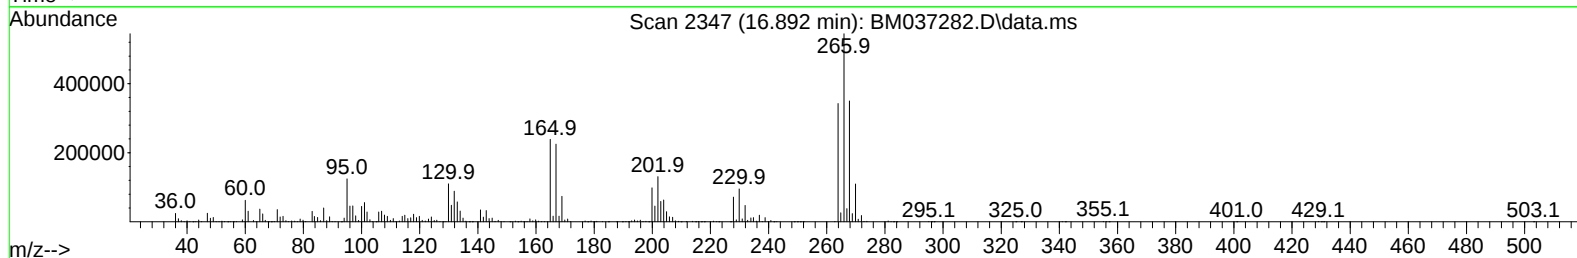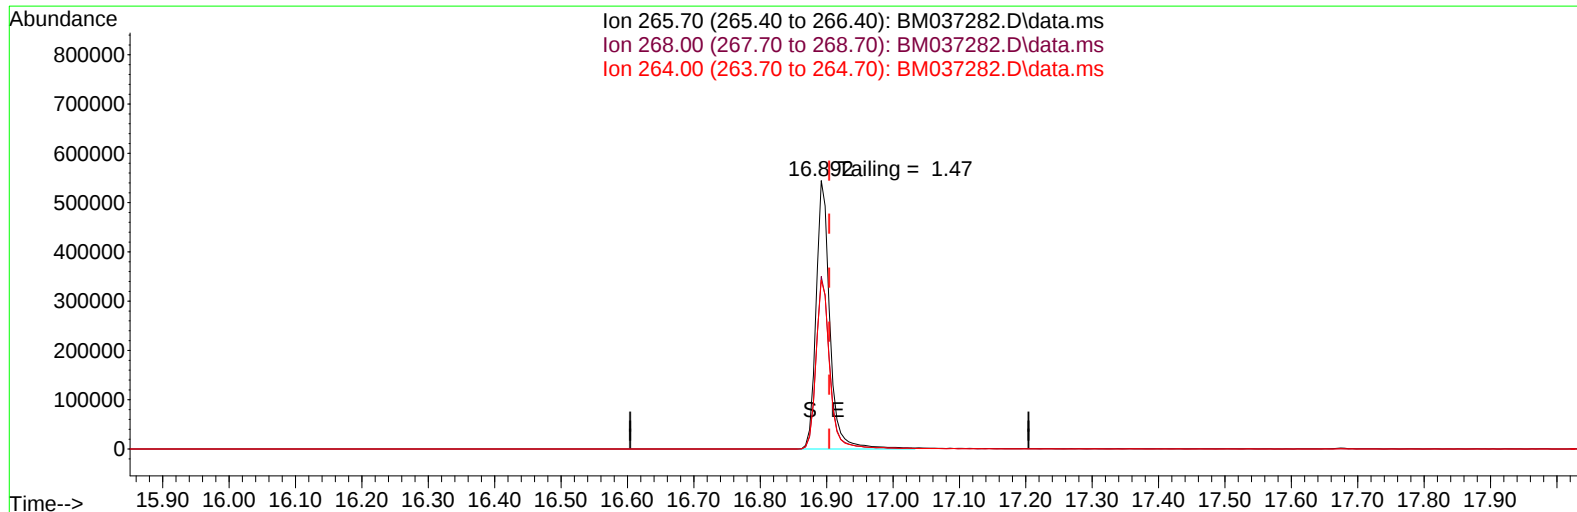

TIC: BM037282.D\data.ms

(70) Pentachlorophenol (C)

16.892min (-0.012) 1812613.78 ng




response 787819

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	64.28
264.00	61.40	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103122\
Data File : BM037282.D
Acq On : 31 Oct 2022 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 01 06:23:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 31 01:34:15 2022
Response via : Initial Calibration

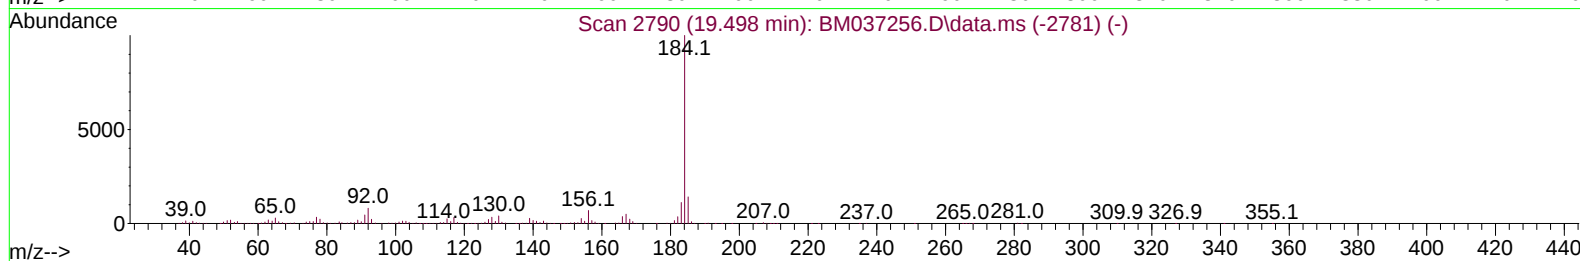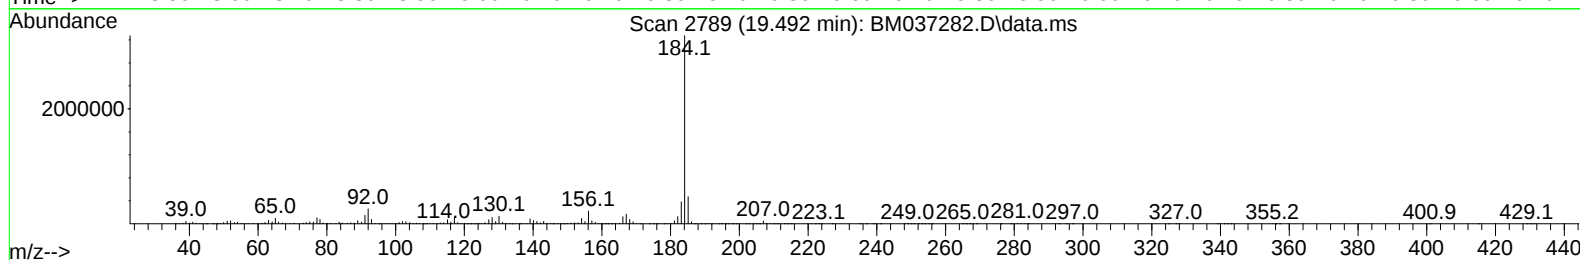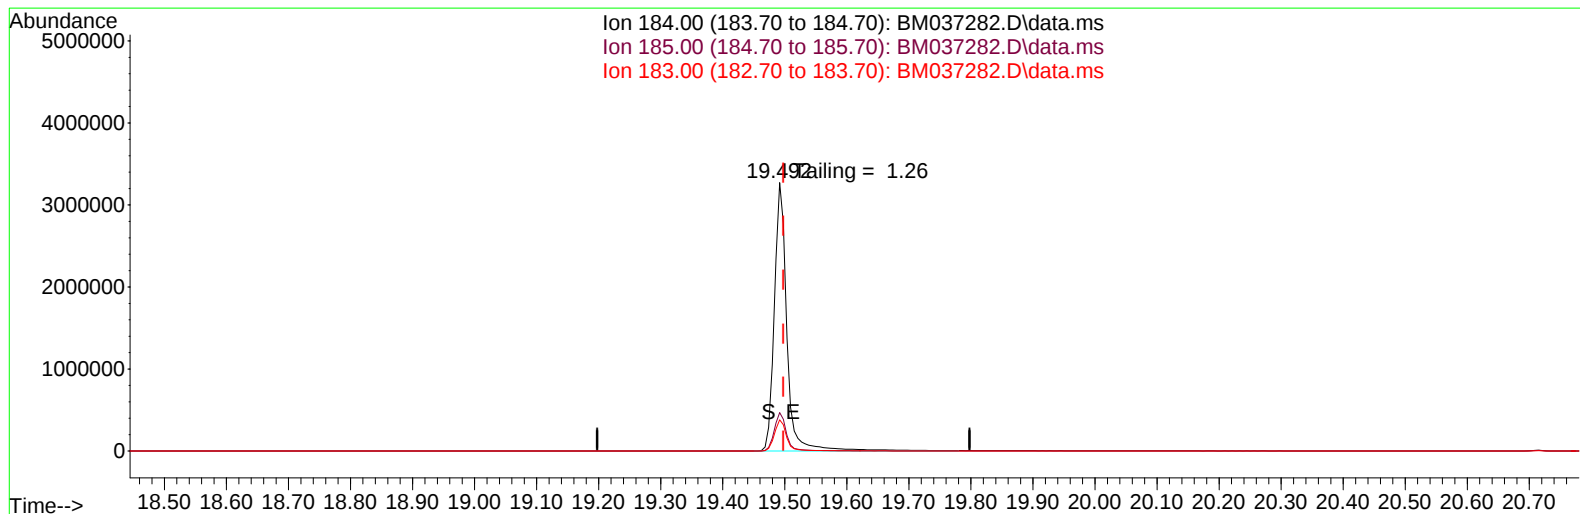

TIC: BM037282.D\data.ms

(77) Benzidine**19.492min (-0.006) 344897.83 ng****response 4628614**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.35
183.00	11.20	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/31/2022	BNA_M	<u>BM037282.D</u>
Compound Name	Response	Retention Time
DDT	2399840	20.715
DDD	33659	20.327
DDE	2917	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36576	2436416	1.50

Instrument :
BNA_M
ClientSampleId :
DFTPP