

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048368.D
 Acq On : 31 Oct 2024 22:02
 Operator : RC/JU
 Sample : P4530-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7H32

Quant Time: Nov 03 07:04:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.712	152	4332	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.495	136	13652	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.353	164	7554	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.195	188	699572	0.400	ng/ul	0.07
17) Chrysene-d12	21.301	240	10770	0.400	ng/ul	0.00
23) Perylene-d12	23.519	264	18896	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	15907	2.990	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.123	152	3508	0.202	ng/ul	-0.02
18) Fluoranthene-d10	19.126	212	8893	0.325	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.484	202	1280	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.364	252	2654	0.044	ng/ul#	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048368.D
Acq On : 31 Oct 2024 22:02
Operator : RC/JU
Sample : P4530-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H32

Quant Time: Nov 03 07:04:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

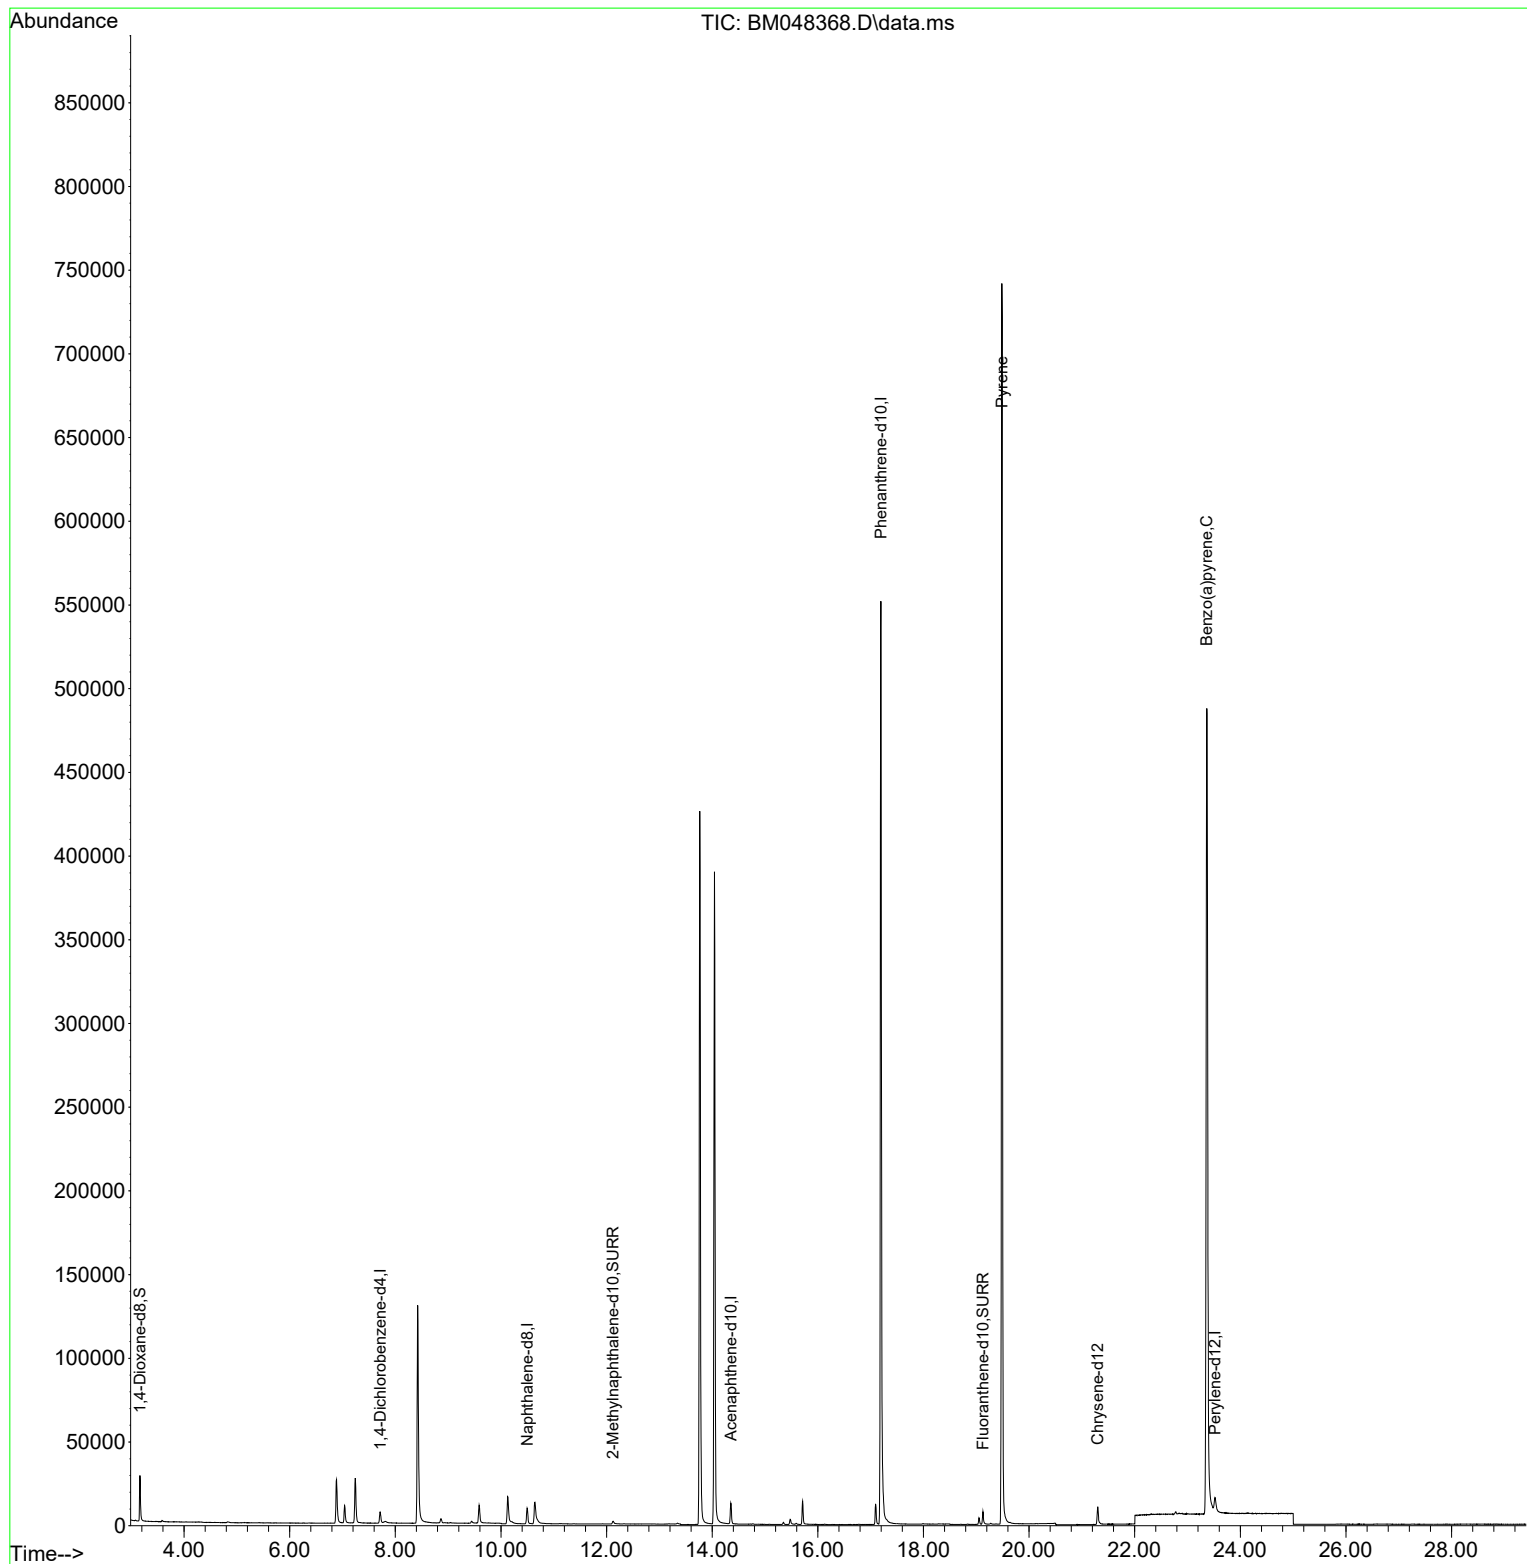

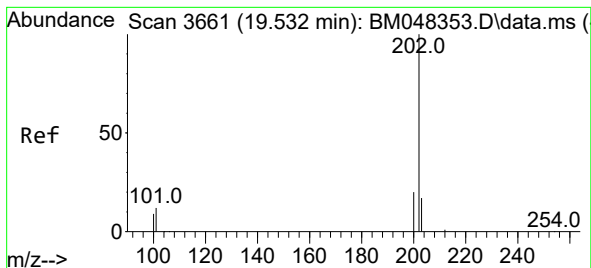

#20

Pyrene

Concen: 0.032 ng/ul

RT: 19.484 min Scan# 3

Delta R.T. -0.048 min

Lab File: BM048368.D

Acq: 31 Oct 2024 22:02

Instrument :





BNA_M

ClientSampleId :

F7H32

Tgt Ion:202 Resp: 1280

Ion	Ratio	Lower	Upper
202	100		
101	141.1	10.0	15.0#
100	1000.5	8.0	12.0#

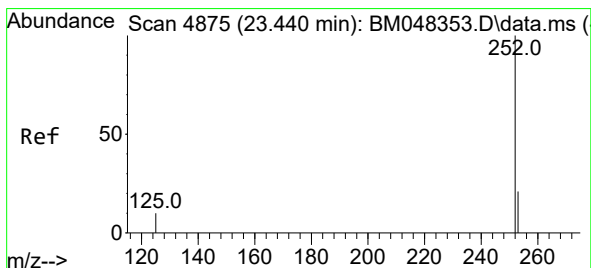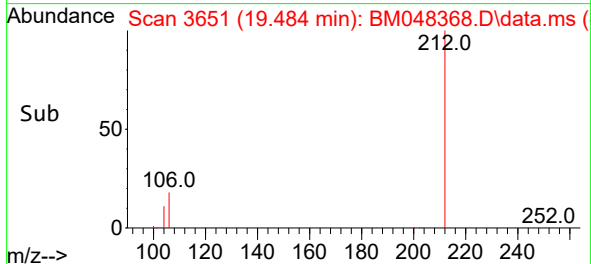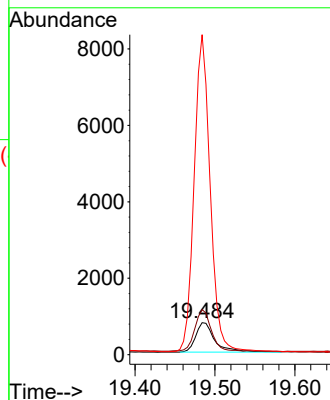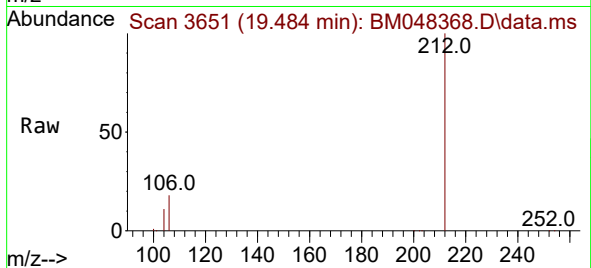

#26

Benzo(a)pyrene

Concen: 0.044 ng/ul

RT: 23.364 min Scan# 4849

Delta R.T. -0.076 min

Lab File: BM048368.D

Acq: 31 Oct 2024 22:02

Tgt Ion:252 Resp: 2654

Ion	Ratio	Lower	Upper
252	100		
253	64.3	27.7	41.5#
125	63.6	21.1	31.7#

