

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048369.D
 Acq On : 31 Oct 2024 22:39
 Operator : RC/JU
 Sample : P4530-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7H33

Quant Time: Nov 03 07:04:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.712	152	4476	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.495	136	14353	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.353	164	7991	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.191	188	854497	0.400	ng/ul	0.07
17) Chrysene-d12	21.295	240	12890	0.400	ng/ul	0.00
23) Perylene-d12	23.519	264	21774	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	19059	3.467	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.118	152	4285	0.235	ng/ul	-0.02
18) Fluoranthene-d10	19.126	212	11073	0.338	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.484	202	1721	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.364	252	3636	0.052	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048369.D
Acq On : 31 Oct 2024 22:39
Operator : RC/JU
Sample : P4530-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H33

Quant Time: Nov 03 07:04:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

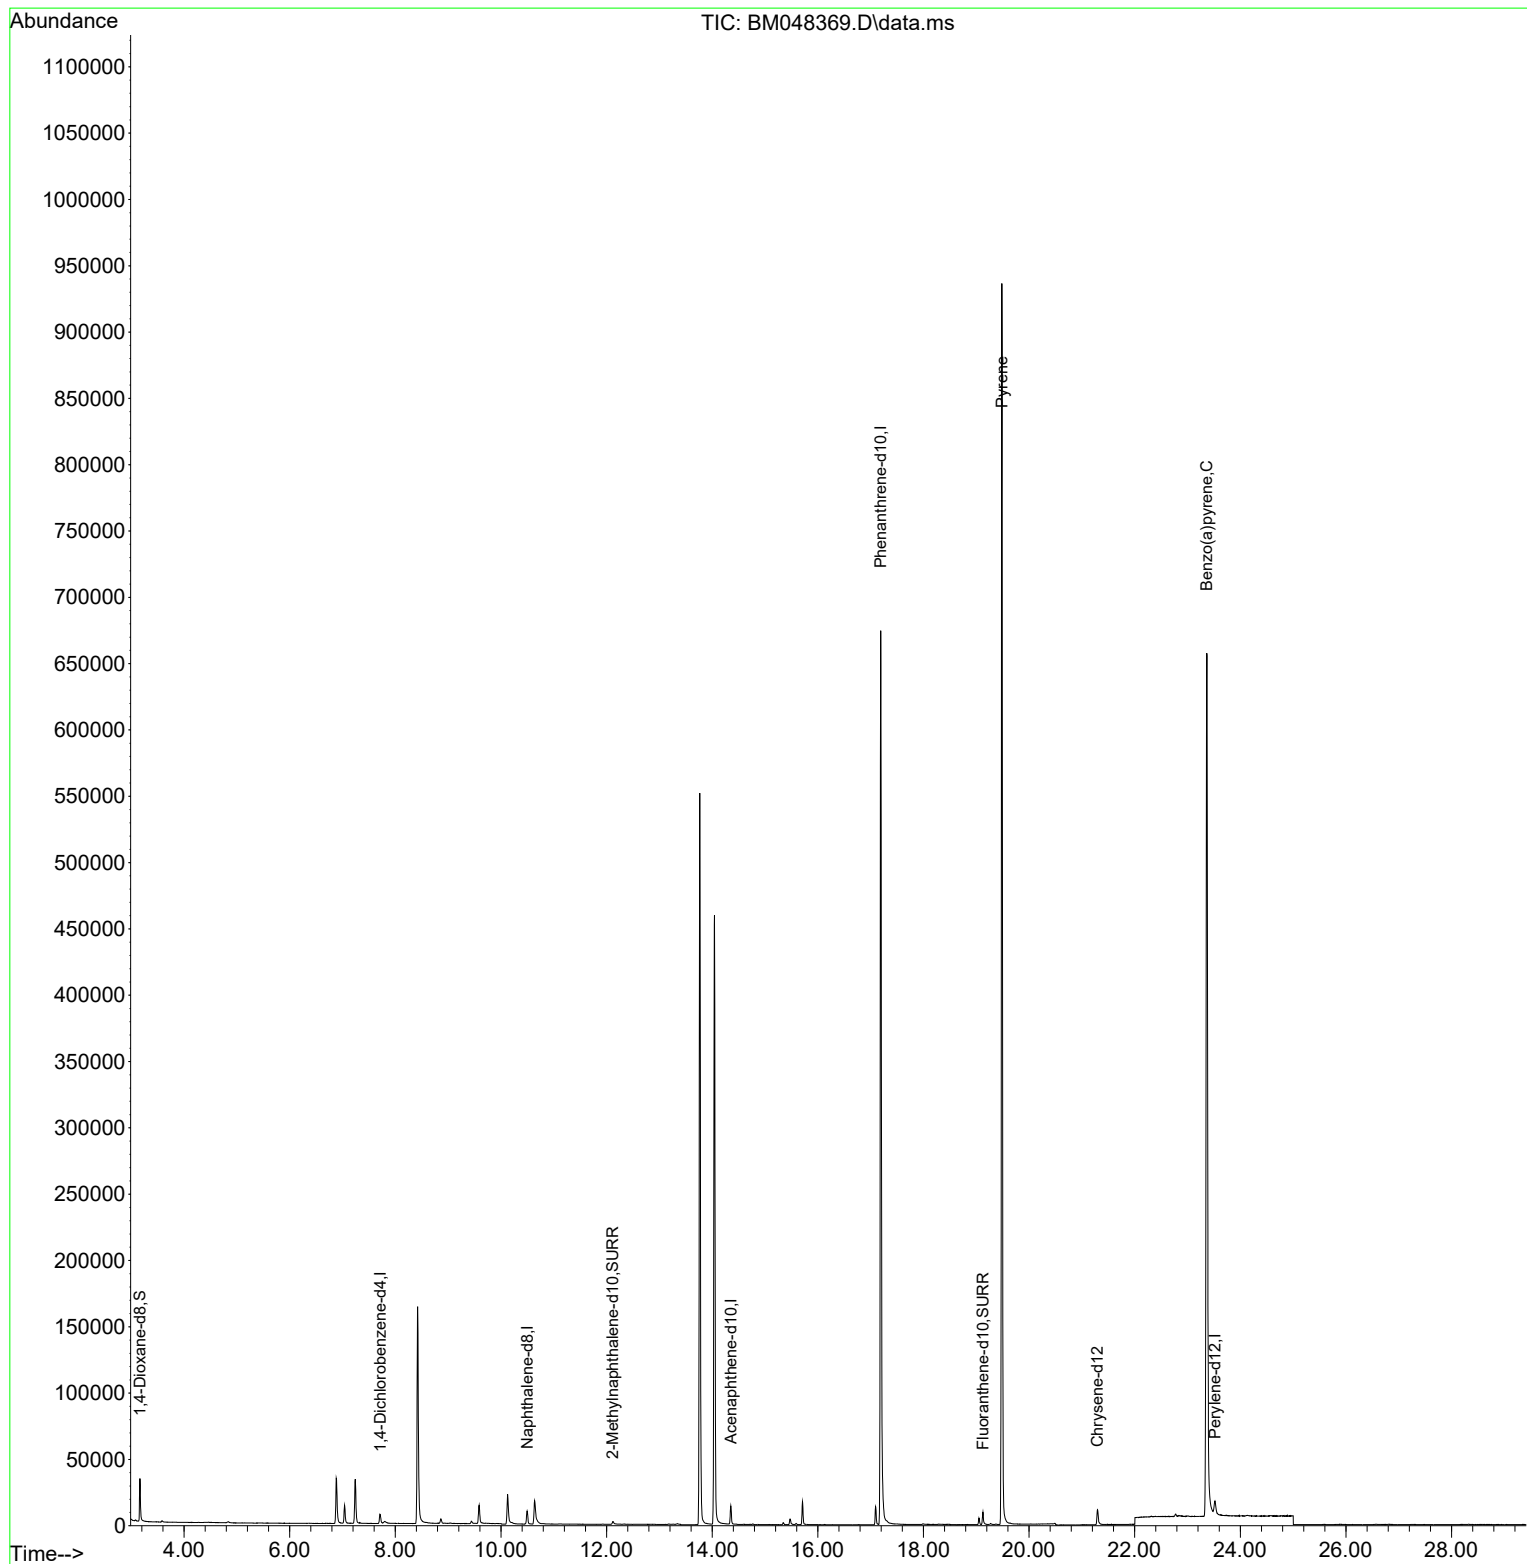

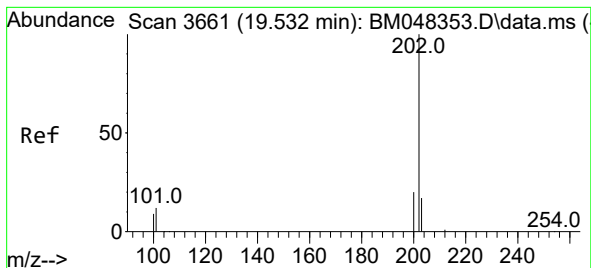

#20

Pyrene

Concen: 0.036 ng/ul

RT: 19.484 min Scan# 3

Delta R.T. -0.048 min

Lab File: BM048369.D

Acq: 31 Oct 2024 22:39

Instrument :

BNA_M

ClientSampleId :

F7H33





Tgt Ion:202 Resp: 1721

Ion Ratio Lower Upper

202 100

101 145.6 10.0 15.0#

100 1026.7 8.0 12.0#

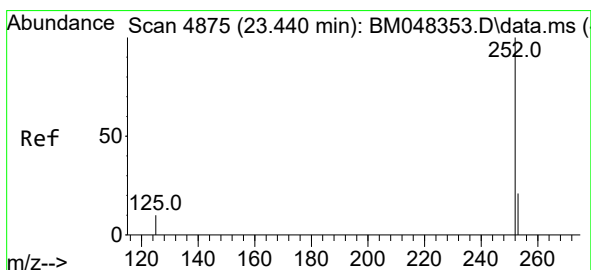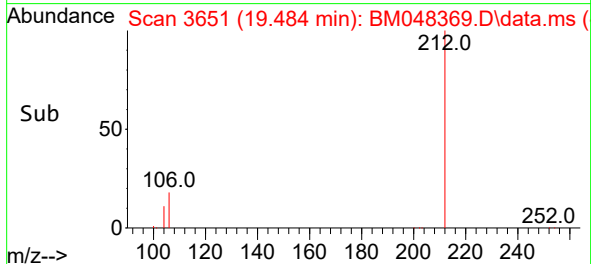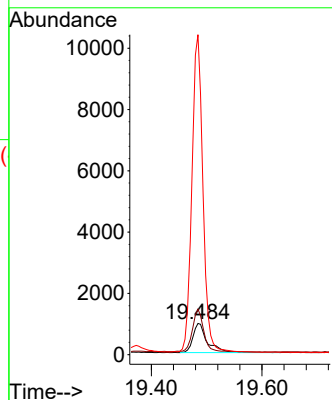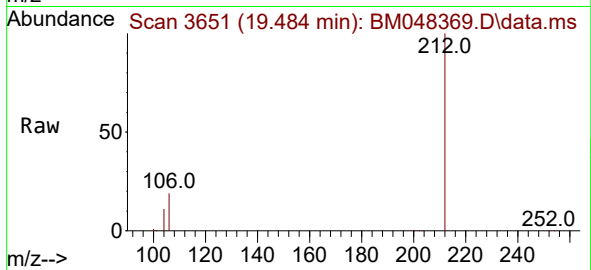

#26

Benzo(a)pyrene

Concen: 0.052 ng/ul

RT: 23.364 min Scan# 4849

Delta R.T. -0.076 min

Lab File: BM048369.D

Acq: 31 Oct 2024 22:39

Tgt Ion:252 Resp: 3636

Ion Ratio Lower Upper

252 100

253 56.9 27.7 41.5#

125 54.7 21.1 31.7#

