

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048374.D
 Acq On : 01 Nov 2024 01:40
 Operator : RC/JU
 Sample : P4530-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7H41

Quant Time: Nov 03 07:04:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.712	152	4476	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.497	136	14301	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.349	164	7676	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.192	188	854902	0.400	ng/ul	0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.29
23) Perylene-d12	23.519	264	18842	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	20233	3.681	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.119	152	4665	0.256	ng/ul	-0.02
18) Fluoranthene-d10	19.123	212	10959	0.000	ng/ul	-0.01
Target Compounds						
					Qvalue	
24) Benzo(b)fluoranthene	22.841	252	1427	0.022	ng/ul#	1
26) Benzo(a)pyrene	23.364	252	3814	0.063	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048374.D
Acq On : 01 Nov 2024 01:40
Operator : RC/JU
Sample : P4530-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H41

Quant Time: Nov 03 07:04:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

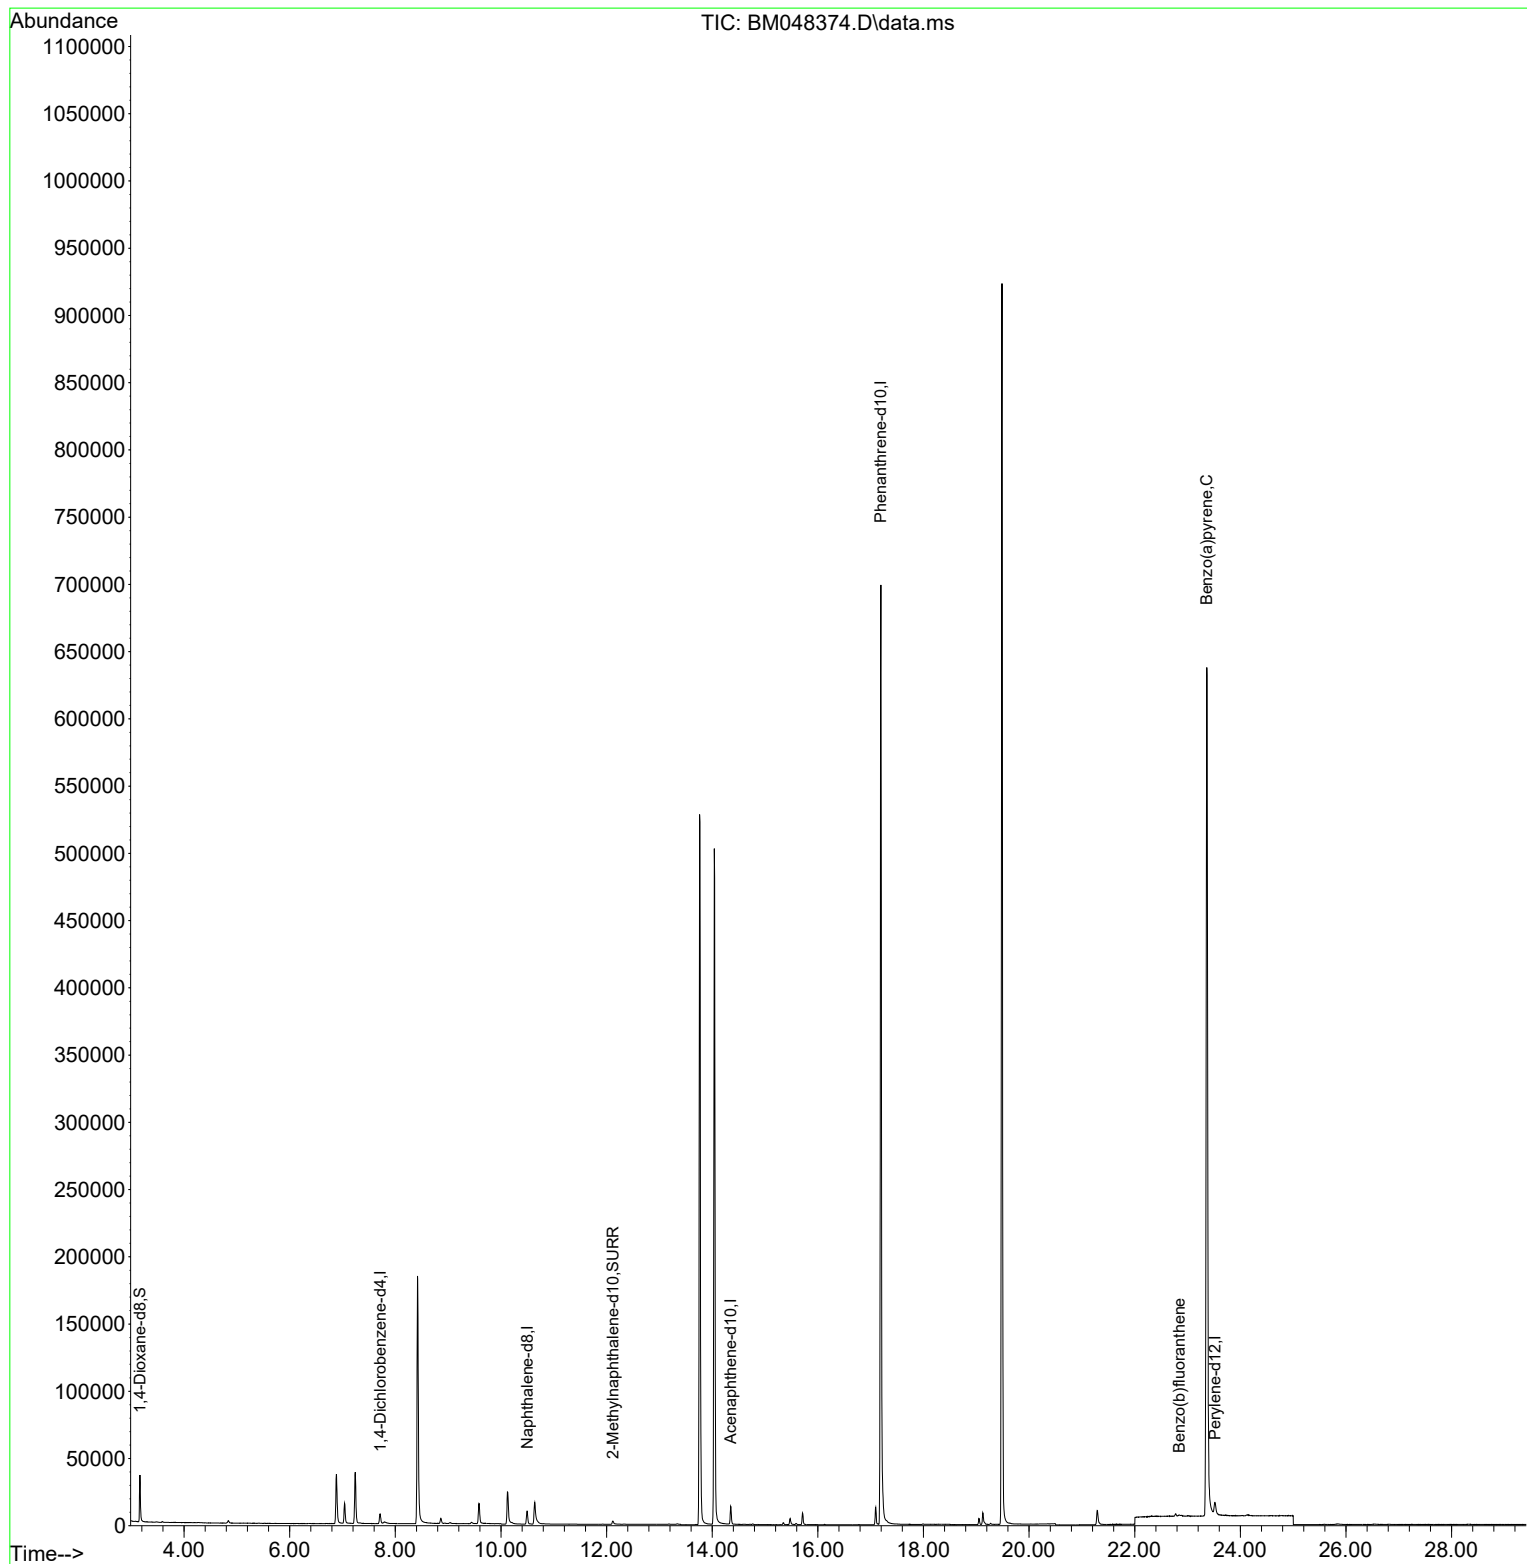

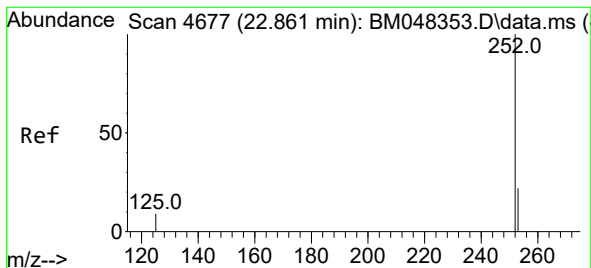

#24

Benzo(b)fluoranthene

Concen: 0.022 ng/ul

RT: 22.841 min Scan# 4

Delta R.T. -0.020 min

Lab File: BM048374.D

Acq: 01 Nov 2024 01:40

Instrument :

BNA_M

ClientSampleId :

F7H41





Tgt Ion:252 Resp: 1427

Ion Ratio Lower Upper

252 100

253 78.7 0.0 59.4#

125 79.3 0.0 38.0#

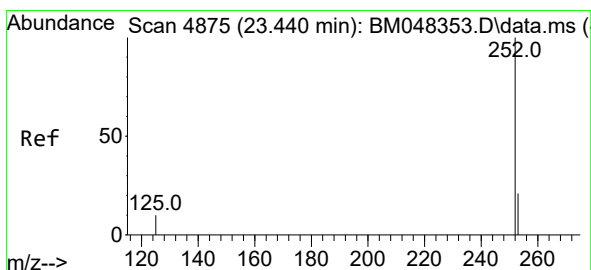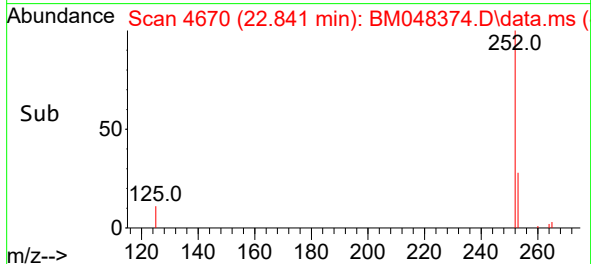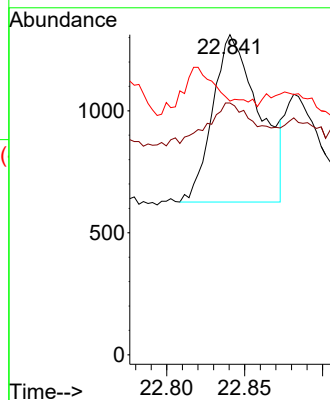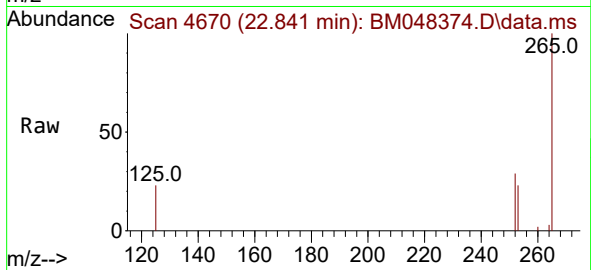

#26

Benzo(a)pyrene

Concen: 0.063 ng/ul

RT: 23.364 min Scan# 4849

Delta R.T. -0.076 min

Lab File: BM048374.D

Acq: 01 Nov 2024 01:40

Tgt Ion:252 Resp: 3814

Ion Ratio Lower Upper

252 100

253 58.5 27.7 41.5#

125 54.9 21.1 31.7#

