

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048377.D
 Acq On : 01 Nov 2024 03:29
 Operator : RC/JU
 Sample : P4530-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7H44

Quant Time: Nov 03 07:05:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	5118	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.495	136	16483	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.353	164	8799	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.191	188	886714	0.400	ng/ul	0.07
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.29
23) Perylene-d12	23.516	264	19589	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	23913	3.804	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.118	152	5371	0.256	ng/ul	-0.02
18) Fluoranthene-d10	19.126	212	11112	0.000	ng/ul	-0.01
Target Compounds						
					Qvalue	
24) Benzo(b)fluoranthene	22.841	252	4061	0.061	ng/ul#	33
25) Benzo(k)fluoranthene	22.841	252	4061	0.051	ng/ul#	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048377.D
Acq On : 01 Nov 2024 03:29
Operator : RC/JU
Sample : P4530-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H44

Quant Time: Nov 03 07:05:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration




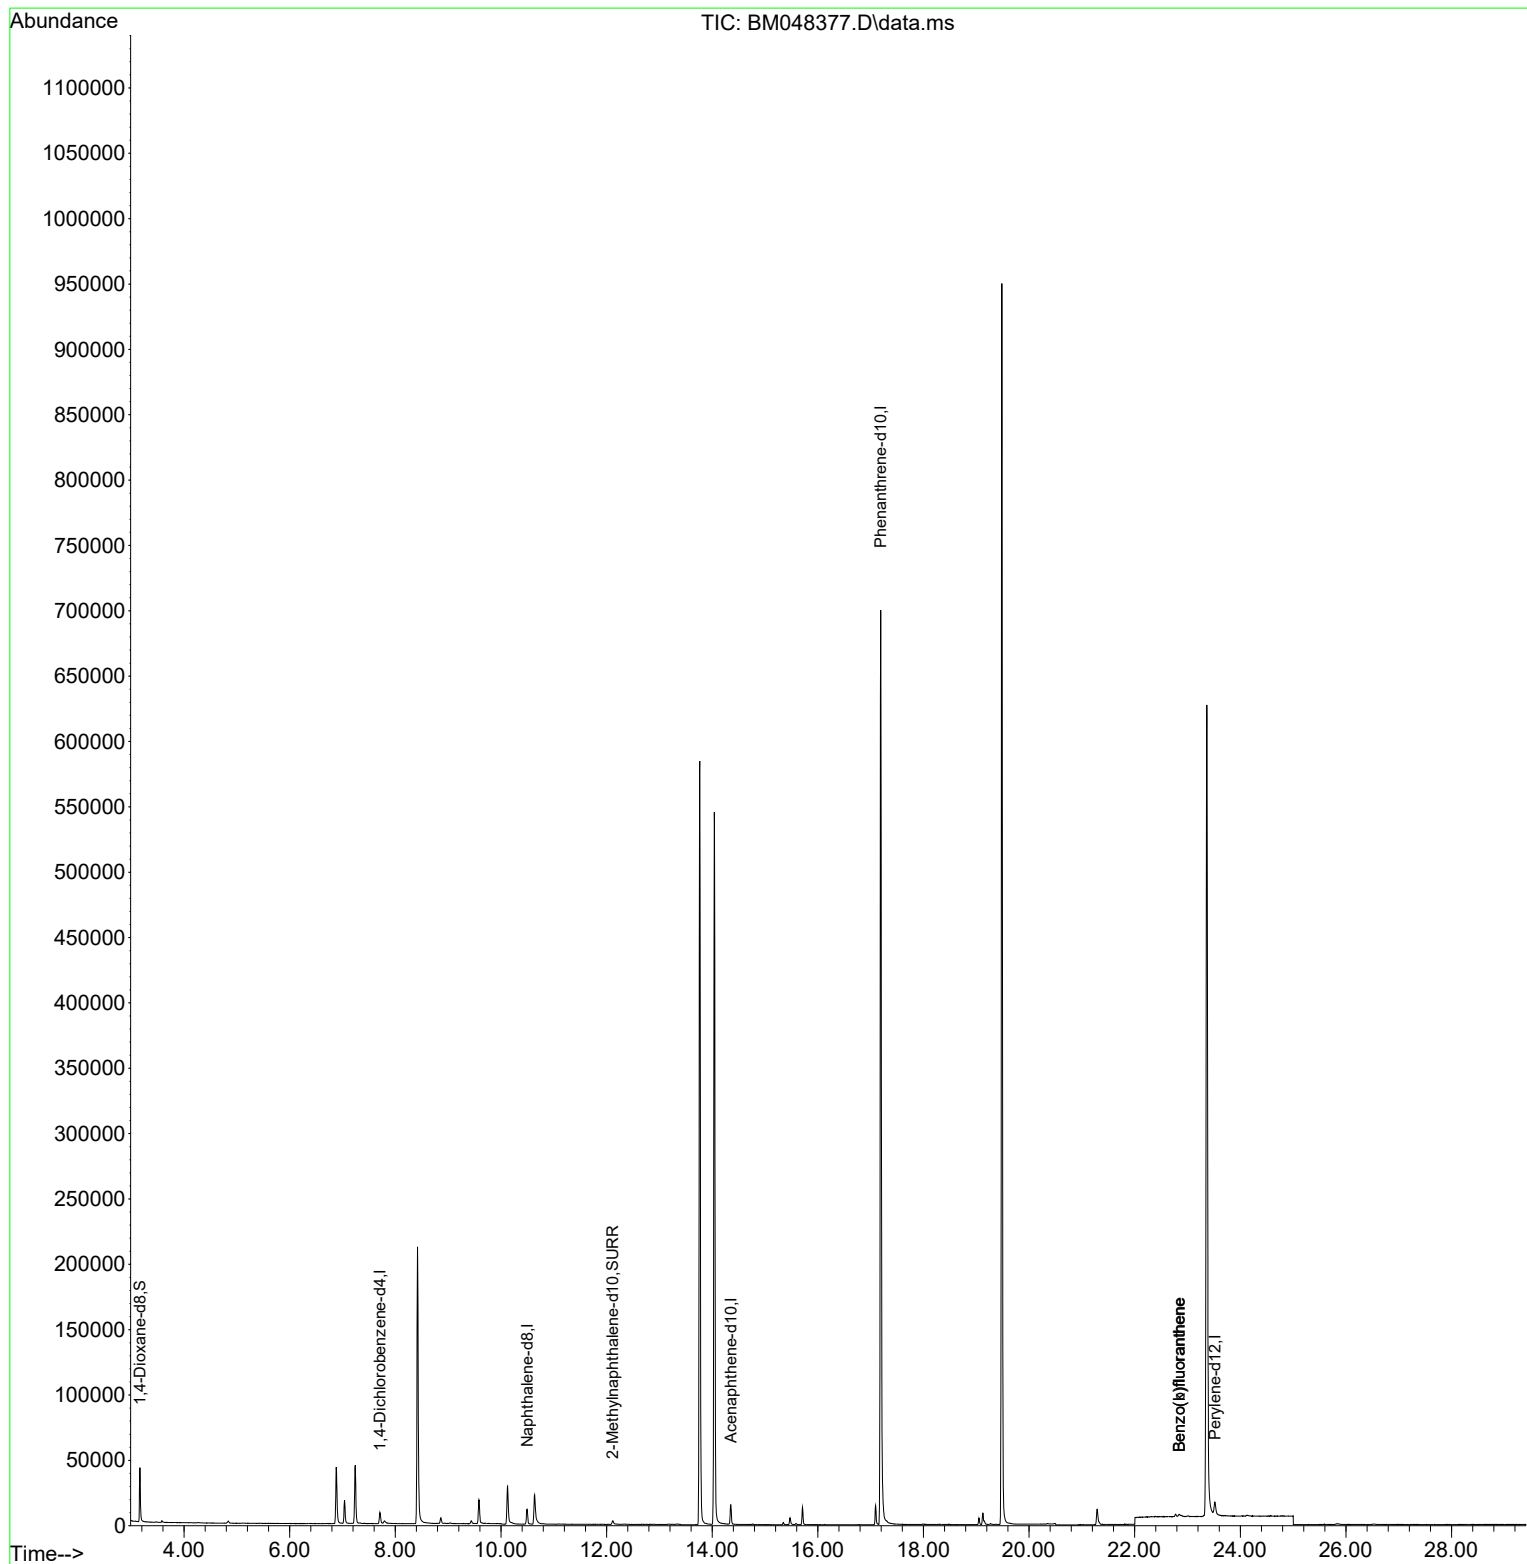


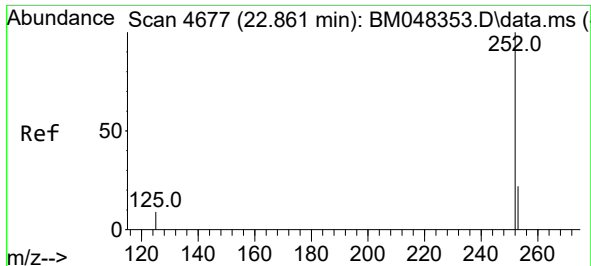

#24
Benzo(b)fluoranthene
Concen: 0.061 ng/ul
RT: 22.841 min Scan# 4670
Delta R.T. -0.020 min
Lab File: BM048377.D
Acq: 01 Nov 2024 03:29

Instrument :
BNA_M
ClientSampleId :
F7H44

Tgt Ion:252 Resp: 4061
Ion Ratio Lower Upper
252 100
253 60.4 0.0 59.4#
125 56.8 0.0 38.0#

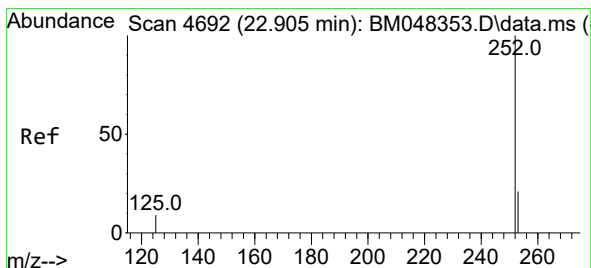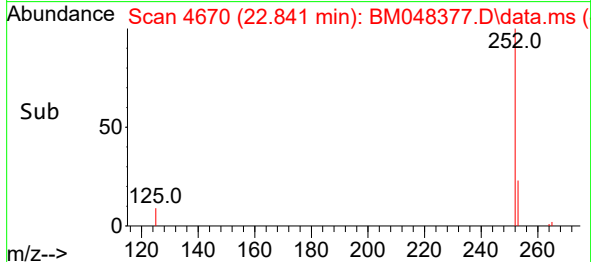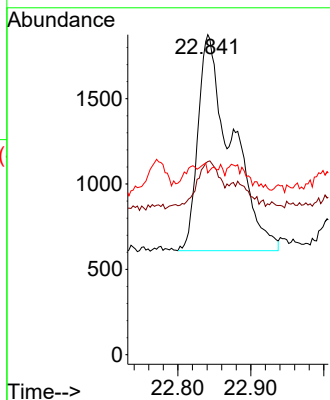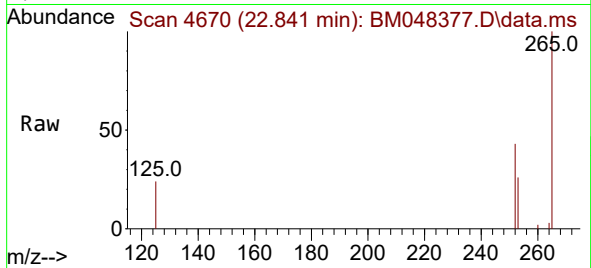

#25
Benzo(k)fluoranthene
Concen: 0.051 ng/ul
RT: 22.841 min Scan# 4670
Delta R.T. -0.064 min
Lab File: BM048377.D
Acq: 01 Nov 2024 03:29

Tgt Ion:252 Resp: 4061
Ion Ratio Lower Upper
252 100
253 60.4 23.4 35.0#
125 56.8 15.3 22.9#

