

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
 Data File : BM048385.D
 Acq On : 01 Nov 2024 08:56
 Operator : RC/JU
 Sample : PB164507BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK507

Quant Time: Nov 03 21:48:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 14:58:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	4577	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.491	136	15075	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.349	164	8283	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.192	188	1129602	0.400	ng/ul	0.07
17) Chrysene-d12	21.303	240	11438	0.400	ng/ul	0.01
23) Perylene-d12	23.516	264	20056	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.160	96	31301	5.568	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.119	152	6422	0.335	ng/ul	-0.02
18) Fluoranthene-d10	19.123	212	13537	0.466	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.485	202	1834	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.361	252	3829	0.059	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103124\
Data File : BM048385.D
Acq On : 01 Nov 2024 08:56
Operator : RC/JU
Sample : PB164507BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK507

Quant Time: Nov 03 21:48:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 14:58:12 2024
Response via : Initial Calibration

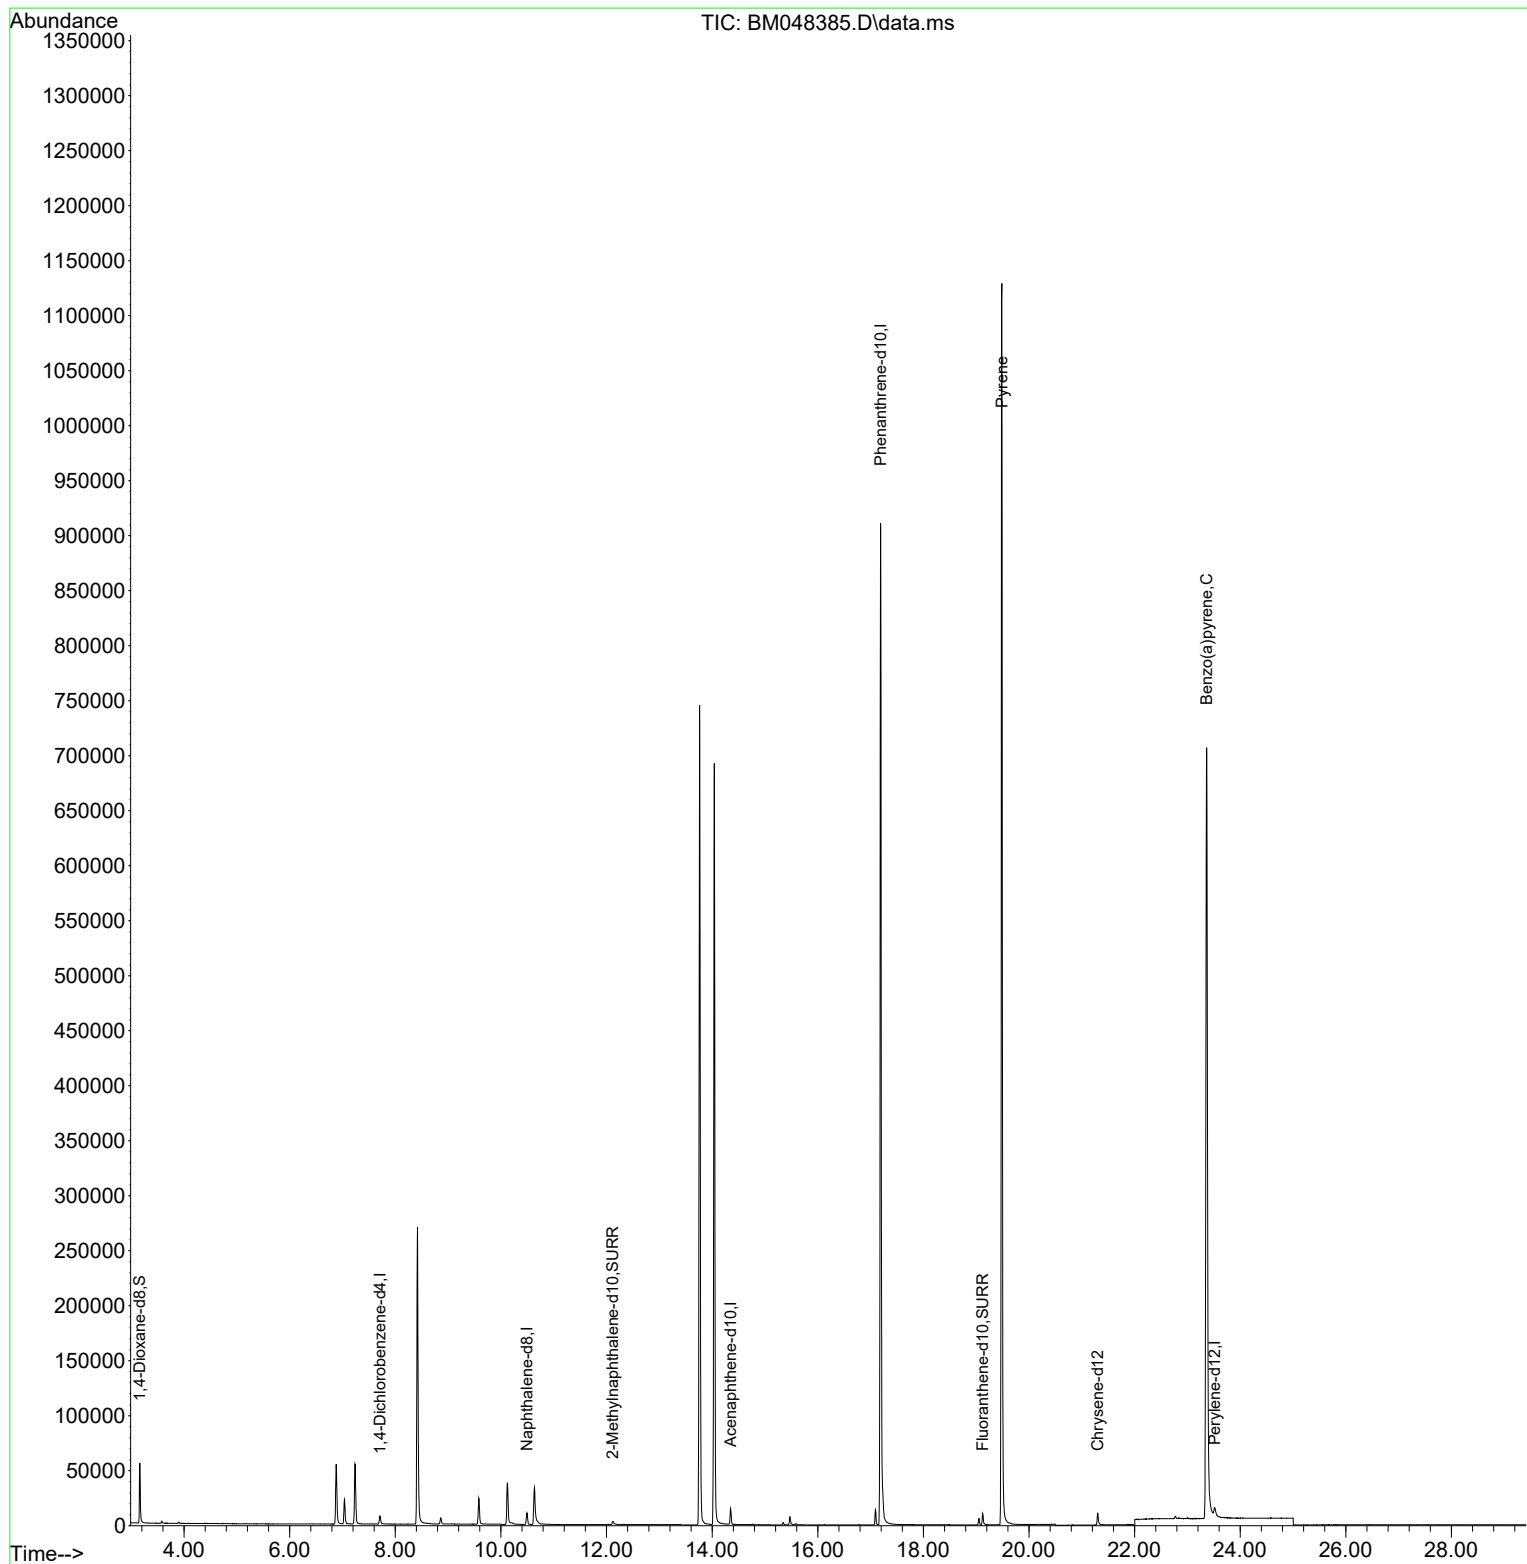

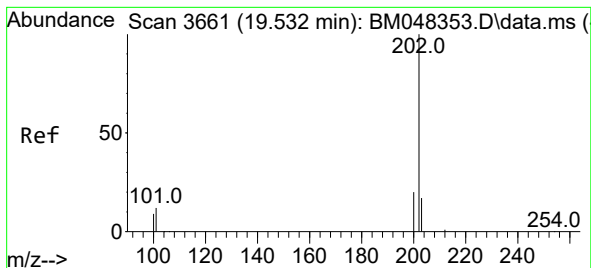

#20

Pyrene

Concen: 0.043 ng/ul

RT: 19.485 min Scan# 3

Delta R.T. -0.047 min

Lab File: BM048385.D

Acq: 01 Nov 2024 08:56

Instrument :

BNA_M

ClientSampleId :

SBLK507





Tgt Ion:202 Resp: 1834

Ion Ratio Lower Upper

202 100

101 134.0 10.0 15.0#

100 932.6 8.0 12.0#

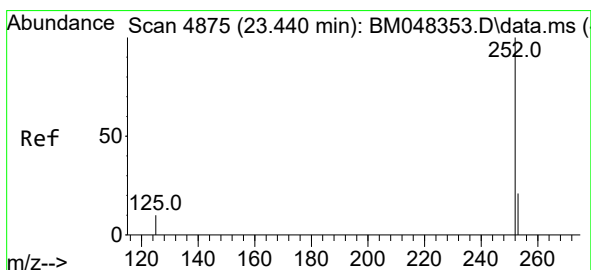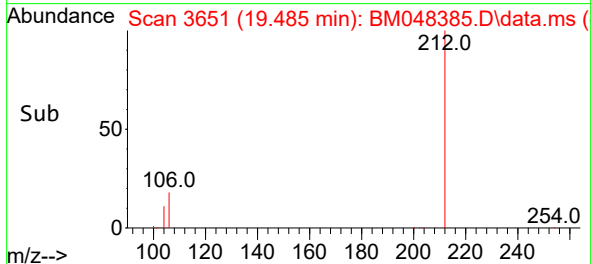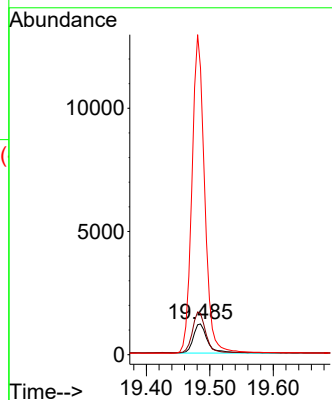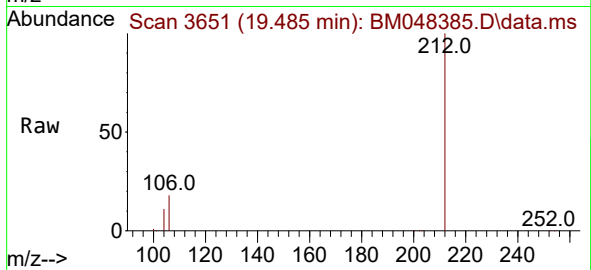

#26

Benzo(a)pyrene

Concen: 0.059 ng/ul

RT: 23.361 min Scan# 4848

Delta R.T. -0.079 min

Lab File: BM048385.D

Acq: 01 Nov 2024 08:56

Tgt Ion:252 Resp: 3829

Ion Ratio Lower Upper

252 100

253 52.7 27.7 41.5#

125 49.0 21.1 31.7#

